

Please type a plus sign (+) inside this box ☒

UTILITY
PATENT APPLICATION
TRANSMITTAL

Attorney Docket No.

GYN-0045

First Named Inventor or Application Identifier

Jörg Priewe

Express Mail Label No.

EL457887031US

Only for new nonprovisional applications under 37 CFR 1.53(b)

APPLICATION ELEMENTS

See MPEP Chapter 600 concerning utility patent application contents.

ADDRESS TO: Assistant Commissioner for Patents
Box Patent Application
Washington, DC 20231

1. ☒ Fee Transmittal Form (attached hereto in duplicate)

2. ☒ Specification [Total Pages]

(Preferred arrangement set forth below)

- Descriptive Title of the Invention
- Cross References to Related Applications
- Statement Regarding Fed sponsored R&D
- Reference to Microfiche Appendix
- Background of the Invention
- Brief Summary of the Invention
- Brief Description of the Drawings (if filed)
- Detailed Description
- Claim(s)
- Abstract of the Disclosure

3. ☒ Drawing(s) (35 USC 113) [Total Sheets 26]

4. Oath or Declaration

- a. ☐ Newly executed (original or copy)
- b. ☒ Unexecuted original
- c. ☐ Copy from a prior application (37 CFR 1.63(d))
(for continuation/divisional check boxes 5 and 16)
- i. ☐ Deletion of Inventor(s)
Signed statement attached deleting inventor(s) named in the prior application, see 37 CFR 1.63(d)(2) and 1.33(b).

5. ☐ Incorporation by Reference
(useable if Box 4c is checked)
The entire disclosure of the prior application, from which a copy of the oath or declaration is supplied under Box 4c, is considered as being part of the disclosure of the accompanying application and is hereby incorporated by reference therein.

- 6. ☐ Microfiche Computer Program (Appendix)
- 7. Nucleotide and/or Amino Acid Sequence Submission (if applicable, all necessary)
 - a. ☐ Computer Readable Copy
 - b. ☐ Paper Copy (identical to computer copy)
 - c. ☐ Statement verifying identity of above copies

ACCOMPANYING APPLICATION PARTS

- 8. ☐ Assignment Papers (cover sheet & document(s))
- 9. ☐ 37 CFR 3.73(b) Statement (when there is an assignee) ☐ Power of Attorney
- 10. ☐ English Translation Document (if applicable)
- 11. ☐ Information Disclosure Statement (IDS)/PTO-1449 ☐ Copies of IDS Citations
- 12. ☐ Preliminary Amendment
- 13. ☒ Return Receipt Postcard (MPEP 503) (Should be specifically itemized)
- 14. ☐ Certified Copy of Priority Document(s) (if foreign priority is claimed)

15. ☐ Other:

- 16. ☐ If a CONTINUING APPLICATION, check appropriate box and supply the requisite information:
Amend the specification by inserting before the first line: -- This is a ☐ Continuation ☐ Divisional
☐ Continuation-in-Part (CIP) of prior application No.: , filed . --
17. For this divisional application, please cancel original Claims of the prior application before calculating the filing fee.

18. CORRESPONDENCE ADDRESS

☐ Customer Number or Bar Code Label or ☒ Correspondence Address below

Name: Audley A. Ciamporcero, Jr., Esq.
Address: Johnson & Johnson
One Johnson & Johnson Plaza
New Brunswick, NJ 08933-7003 USA


19. TELEPHONE CONTACT

Please direct all telephone calls or telefaxes to Verne E. Kreger, Jr. at:
Telephone: (732) 524-1239 Fax: (732) 524-2808

19. SIGNATURE OF APPLICANT, ATTORNEY, OR AGENT REQUIRED

NAME Verne E. Kreger, Jr. Reg. No. 35231

SIGNATURE



DATE

June 7, 2000

IN THE UNITED STATES
PATENT AND TRADEMARK OFFICE



Applicant: Priewe et al.

For : Method and Apparatus for Adjusting Flexible Areal
Polymer Implants

Express Mail Certificate

"Express Mail" mailing number: EL457887650US

Date of Deposit: June 7, 2000

I hereby certify that this complete application, including specification pages, claims, and informal drawings, is being deposited with the United States Postal Service "Express Mail Post Office to Addressee" service under 37 CFR 1.10 on the date indicated above and is addressed to the Assistant Commissioner for Patents, Washington, D.C. 20231.

A Combined Declaration and Power of Attorney will be submitted to the United States Patent and Trademark Office upon receipt of the U.S. Serial Number for this patent application.

Alwin M. Haywood

(Typed or printed name of person mailing paper or fee)

(Signature of person mailing paper or fee)

09589242-060700

UNITED STATES PATENT APPLICATION FOR:

**METHOD AND APPARATUS FOR ADJUSTING FLEXIBLE AREAL POLYMER
IMPLANTS**CROSS REFERENCE TO RELATED APPLICATION

The present invention claims the benefit of earlier-filed United States provisional patent application, serial number 60/138,231, filed on June 9, 1999, which is hereby incorporated by reference in its entirety herein.

BACKGROUND OF THE INVENTION

The present invention relates generally to a minimally invasive approach to adjust a flexible areal polymer implant for supporting an anatomical structure and further relates to an approach especially useful for use with implants that support the urethra for treating female urinary incontinence.

Women account for more than 11 million of incontinence cases. Moreover, a majority of women with incontinence suffer from stress urinary incontinence (SUI). Women with SUI involuntarily lose urine during normal daily activities and movements, such as laughing, coughing, sneezing and regular exercise.

SUI may be caused by a functional defect of the tissue or ligaments connecting the vaginal wall with the pelvic muscles and pubic bone. Common causes include repetitive straining of the pelvic muscles, childbirth, loss of pelvic muscle tone, and estrogen loss. Such a defect results in an improperly functioning urethra. Unlike other types of incontinence, SUI is not a problem of the bladder.

Normally, the urethra, when properly supported by strong pelvic floor muscles and healthy connective tissue, maintains a tight seal to prevent involuntary loss of urine. When a woman suffers from the most common form of SUI, however, weakened muscle and pelvic tissues are unable to adequately support the urethra in its correct position. As a result, during normal movements when pressure is exerted on the bladder from the diaphragm, the urethra cannot retain its seal, permitting

urine to escape. Because SUI is both embarrassing and unpredictable, many women with SUI avoid an active lifestyle, shying away from social situations.

United States Patent 5,112,344 describes a method and apparatus for treating female incontinence. The surgical instrument for the application of a
5 filamentary element into the body comprises a tubular shaft having a handle at one end and a flexible needle slidably receivable in the shaft and adapted at one end to receive a filamentary element. The method of treating female incontinence comprises looping a filamentary element between the wall of the vagina and the
10 rectus abdominis sheath in the anterior wall of the abdomen whereby it passes to each side of the urethra, adjusting the loop to bring the vaginal wall and the urethra into the correct spatial relationship to the pubis allowing the development of scar tissue between the vaginal wall and the anterior wall of the abdomen pubic symphysis and removing the filamentary element.

United States Patent 5,899,909 discloses a surgical instrument comprising a
15 shank having a handle at one end and connecting means at the other end to receive, one at a time, two curved needle-like elements which are connected at one end to one end of a tape intended to be implanted into the body. In practice, the tape is passed into the body via the vagina first at one end and then at the other end at one side and the other, respectively, of the urethra to form a loop around the
20 urethra, located between the urethra and vaginal wall. The tape is extended over the pubis and through the abdominal wall and is tightened. The tape ends are cut at the abdominal wall, and the tape is left implanted in the body. U.S. patent no. 5,899,909 is incorporated herein by reference.

While implanting a tape, it is often difficult to determine the most suitable
25 amount of support to provide to the urethral structure. An optimal amount of support is defined as that which provides relief from incontinence and simultaneously provides for normal micturition. Even if the most optimal amount of support is provided during implantation, it is possible that the surrounding tissues will change during the healing process or simply due to aging. As a result,
30 the optimal amount of support is subject to change.

European Patent 0941 712 A1, José Gil-Vernet Vila, describes an approach to adjusting urethral support by use of an expandable container implanted remotely from the urethra and connected to a mesh supporting the urethra. While this provides adjustment capabilities, the associated surgical procedure is invasive and complex. The container is also complex and requires features to assure that the suspending threads are not abraded. The container is preferably located in adipose tissue in the abdominal region. The container's location exposes it to distortion whenever there are external forces applied to the abdominal area. This in turn is expected to transiently change the degree of support to the urethra whereas it is desirable to provide a fairly constant level of support. Since the mesh support is directly in contact with the urethra, the fluctuations of support to the urethra can become irritating to the surrounding tissue.

United States Patent No. 6,042,534, Gellman et al., describes the use of a visual indicator that may be radiopaque. However, there is no specific description of how to achieve this effect and makes no mention of its use with a tape support device. Further, the purpose of this indicator is solely for assessment of the relative position of the sling used to support the urethra. Gellman is silent with respect to the need to adjust the sling after it is in place.

United States Patent No. 5,611,515, Theodore V. Benderev et al., describes the use of a suture tensioning devices in conjunction with bladder neck suspension. These tensioners are used to adjust the tension on sutures used to hold a supportive sling in place on the bladder neck. Prior to tying, sutures are appropriately tensioned by advancing the suture around a suture tensioner and tying in a conventional manner. Thereafter, the suture tensioner is removed and the surgical site prepared and closed in a conventional manner. While this technique is fine for establishing the initial tension to the sling, it does not allow for post implantation adjustment. Also, this approach is fine where the sling is suspended with sutures or other filament means. However, such tensioning

devices are unsuitable for tapes implanted such as those associated with the GYNECARE TVT Tension-Free Support for Incontinence.

International Patent WO 98/31301 discloses an implantable continence device that consists of a hydraulic and mechanical component.

Therefore there is a need to be able to adjust the level of support to the urethra in a less complicated manner and with no urethra-mesh contact. Further, the adjustment should be located in close proximity to where the support is needed.

The present invention discloses devices and methods for adjusting the support of internal anatomical organs both during and after implantation. In particular, the invention is intended to be especially useful for use with implants that support the urethra.

SUMMARY OF THE INVENTION

The invention overcomes the deficiencies of the prior art and provides for an improved apparatus and method for adjusting the level of support provided to an anatomical structure by an implanted tape. The invention finds particular benefit to the treatment of female urinary incontinence.

In particular the invention is useful with system for the treatment of female stress urinary incontinence. The system provides a surgical instrument comprising a handle at one end and connecting means at the other end to receive, one at a time, two curved needle-like elements, each of which has a modified tip. The needle may have a constant or varying diameter. Each needle connects at one end to separate ends of a tape intended to be implanted within the body. In practice, a first end of the tape is passed, via one of the curved needles, into the body via the vagina at one side of the urethra. The needle and first end of the tape pass over the pubis and through the abdominal wall. The second needle element connects to the second end of the tape and passes into the body via the vagina at the opposite site of the urethra from the first end of the tape thereby forming a loop or sling around the urethra with the tape. The second end of the tape is extended over the pubis

and through the abdominal wall. The tape ends are cut at the abdominal wall, and the tape is left in the body.

The invention further provides for a single curved needle element having a modified tip. The needle may have a constant or varying diameter and further provides for a easy attachment means enabling the surgeon to connect both the first and second tape ends to the single needle to perform the above-stated procedure.

In both embodiments, the invention provides for devices and methods for adjusting the level of support provided to the urethra by an implanted tape. Two approaches are offered. One relates to the use of bulking agents, both contained and directly injected into surrounding tissues. In this approach, detectable markers are provided to guide the clinician during the injection process. The second approach offers mechanical means of adjusting the effective length of supporting arms of a tape used to support the urethra. These devices include threadedly adjustable constructions.

The object of the invention is to provide a method for adjusting the level of support to an anatomical structure offered by an implanted tape.

An advantage of the invention is that it provides for continual adjustment capabilities to an implanted tape for supporting an anatomical structure.

These and other features and advantages of the present invention will become apparent from the following more detailed description, when taken in conjunction with the accompanying drawings which illustrate, by way of example, the principles of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

FIGURE 1 is a view of the needle for use with the tape mesh;

FIGURE 2a is a side view of two needles and a tape interconnecting the needles;

FIGURE 2b-d are alternate embodiments of the tape and connecting means between the tape and needle;

FIGURES 3a-g embodiments of means for attaching the tape to the needle;

FIGURES 4a-f are alternate embodiments providing an expandable container associated with the tape mesh;

FIGURES 5a-c are alternate embodiments for providing mechanical adjusting means to the tape mesh;

FIGURES 6a-h illustrate diagrammatically several surgical steps of the method utilizing two needles according to the invention to treat SUI;

FIGURES 7a-h illustrate diagrammatically surgical steps of the method utilizing one needle according to the invention to treat SUI;

FIGURE 8 is diagrammatic representation illustrating direct bulking between the tape and urethra; and

FIGURE 9 is a representation of a detectable target ring implanted in the tape.

DETAILED DESCRIPTION OF THE INVENTION

Before explaining the present invention in detail, it should be noted that the invention is not limited in its application for the treatment of female incontinence or use to the details of construction and arrangement of parts illustrated in the accompanying drawings and description, because the illustrative embodiments of the invention may be implemented or incorporated in other embodiments, variations and modifications, and may be practiced or carried out in various ways.

Furthermore, unless otherwise indicated, the terms and expressions employed herein have been chosen for the purpose of describing the illustrative embodiments of the present invention for the convenience of the reader and are not for the purpose of limiting the invention.

The invention discloses an apparatus and method for treating SUI. A tape is passed through pelvic tissue and positioned underneath the urethra, creating a supportive sling. The tape provides a structure means for tissue ingrowth and thereby provides a newly created body tissue supporting means for the urethra. When pressure is exerted upon the lower abdomen, such as during a cough or

sneeze, the tape provides support to the urethra, allowing it to keep its seal and prevent the unwanted discharge of urine.

Referring to Figs. 1 and 2a, the surgical instrument comprises a needle-like element 10 that attaches to a mesh tape 12. Needle element 10 defines a certain radius R to perform the surgical procedure discussed herein. The distal end of needle element 10 terminates at a conical section 14 having a tip 16. Alternate configurations, such as a blade-like, arrow or burr tips are also possible. Preferably, tip 16 is blunt, wherein the tip 16 has a radius of about 0.6 millimeters. A blunt tip is preferred since it is less likely to stick in bone or penetrate bladder wall tissue or blood vessel wall tissue as will be appreciated from the method of implanting the tape as described below.

The proximal end of needle 10 terminates in an attachment segment 20 that is adapted to mate and lock into a handle 411 as disclosed in US patent no. 5,899,909, previously incorporated herein by reference.

Disposed between cone portion 14 and segment 20 is a curved shaft segment 18 having a distal end 17 and a proximal end 19. The shape of shaft 18 extends substantially a quarter of a circle in order to follow substantially the profile of the pubis between the vagina and the abdominal wall. For the purposes of the method as will be discussed in more detail below, shaft 18 has a preferred radius R of about 106 millimeters. The diameter of the curved shaft segment 18 may be constant or the diameter of segment 18 transitions from a smaller diameter at distal end 17 to a larger diameter at proximal end 19. The minimum diameter of distal end 17 may be as small as 0.5mm due to the minimal stresses at this point. The minimal diameter of proximal end 19 is about 4mm. Preferably, the diameter at the proximal end is about 6 mm, and reduces in a continuous manner to a diameter of about 3 mm at the distal end 17. This design takes into account, that in the method to implant the tape 12, the bending stresses are lowest at distal end 17, while the bending stresses are highest at the proximal end 19. Stated differently, during the procedure, the inner bending moment at distal end 17 is negligible, while the inner bending moment at the proximal end 19 is substantial.

Needle 10 is preferably has a circular cross section and is made from a material that is compatible with the human body. It is also preferred that needle 10 is made from a material that can be autoclaved to enable multiple surgical procedures of needle 10. Preferably, needle 10 is made from 303 stainless steel. The surface of shaft 18 may be smooth, preferably polished, to facilitate penetration of the soft tissue. Alternatively, the surface of needle 10 may have a somewhat rougher surface. A rougher surface would result in slightly additional tissue trauma, which in turn stimulates fibroblast activity around the tape 12.

Needle 10 may be manufactured as a single, continuous unit, or alternatively, curved portion 18 may be manufactured separately from linear portion 20. In this manner the two pieces would attach using any conventional attaching means, such as, screwing, or other conventional means as is known to those skilled in the art.

Referring to Figs. 2a-d, tape 12 comprises any tissue-compatible synthetic material, or any natural material, including, but not limited to, autologous, allograft, xenograft, a tissue engineered matrix, or a combination thereof. An exemplary synthetic material is PROLENE® polypropylene mesh, a mesh having a thickness of 0.7 mm and openings of about 1mm manufactured by Ethicon, Inc., Somerville, New Jersey, U.S.A. This material is approved by the U.S. Food and Drug Administration for implantation into the human body. A still further embodiment of the tape 12 is a combination of a synthetic material 11 and a natural material 13 centered between the synthetic material 11 as shown in Figs. 2b-c. A still further embodiment of the tape 12 includes a combination of synthetic material 11 and natural material 13, whereby the natural material is placed over or incorporated within a generally central portion of the synthetic material 11. One advantage of the tape configurations is that natural material 13 is along the center region of tape 12 so that after installation of tape 12, natural material 13 is positioned below the urethra and eliminates possible erosion issues at the interface of the urethra and tape. Natural material 13 may be connected to the synthetic material 11 by means of sewing, a bio-compatible glue, cell culturing techniques or other known means.

Tape 12 may be of any convenient shape that suits the intended purpose of the invention. An exemplary width is about 1 cm and the length would be dependent upon the size of the female undergoing the procedure. Tape 12 may be single or double ply, generally planar in structure, or tubular (Fig. 2d) to provide additional supporting strength and more surface area on which tissue fibers may attach.

Moreover, tape 12 may consist of different types of material, such as a bioabsorbable and non-bioabsorbable material. Tape 12 may also be coated with an antimicrobial additive to prevent or minimize infection and a lubricous coating, for example, a bioabsorbable hydrogel, to facilitate the tape passing through the tissue as discussed below. Preferably, tape 12 is covered by a removal plastic sheath as disclosed in U.S. patent no. 5,899,909. The tape may also be made radio-opaque and/or of a contrasting color to the body tissue to allow for future diagnostic visualization.

Referring to Figs. 4a-f, tape 12 is further modified to include an expandable container or chamber 100 positioned on the tape 12 so the chamber 100 is located between the urethra and tape surface after the surgical procedure, discussed below. The container 100 serves to limit migration and/or resorption of the bulking agent. Further, the chamber 100 expands or contracts by either injecting into or extracting bulking material from the chamber 100.

The container 100 may be made of a biocompatible material such as a hydrogel (i.e., crosslinked methacrylic-PEG esters, PHEMA, PMMA, phospholipid-like methacrylic polymers, radiation crosslinked PEO or PEG), polypropylene, polyester, silicone, or polyurethane. The container may be an integral part of the tape or may be slidably attached so that its position is such that it will work in unison with the tape in supporting the urethra. This should be near the center of the mesh so that after implantation, container 100 is positioned below the urethral area. Optionally, container 100 has a touchable internal valve element 101 to permit the surgeon to palpate the area prior to injecting or removing the bulking agent. Alternatively, the bulking agent may be injected and removed via a two-way external port 102. When a bulking agent is injected into container 100 the

tissue between mesh and urethra will expand. This results in two effects; a simple vertical lifting due to expansion and a vertical lifting due to stretching the outside of the mesh. A suitable bulking agent may be water or saline.

Preferably, container 100 has no voids when empty and has a height of about 0.5 cm to about 2 cm and a length from about 2 cm to about 4 cm. Container 100 may be an cube-like expandable element of Fig. 4a, or a dome-shape of Fig. 4b. The container 100 also includes a foot portion 103 suitable for attachment to tape 12. Attachment may be achieved by incorporating the tape into the foot with the hydrogel being on both sides of the tape as shown in Fig. 4b. Foot portion 103 is preferred when the tape is a polypropylene mesh since polypropylene materials do not accept adhesive material. This configuration is preferred because container 100 increases the effective bending stiffness of the tape 12 in the area of the container's attachment.

Alternatively, container 100 may comprise two chambers 100a, 100b in fluid communication with each other. Alternatively, the two chambers 100a, 100b may be separate and effectively two containers. However, they may be linked together by a common injection port. This configurations allows for tissue expansion both underneath and lateral to the urethra.

The addition of container 100 to the mesh 12 acts to increase the effective bending stiffness of the mesh 12 in the area of the attachment of container 100. The increased bending stiffness provides additional support to the urethra when the mesh 12 is implanted. The bending stiffness further increases when the container 100 is filled with bulking agents

If container 100 is semi-permeable, the injected bulking agent can be designed to take advantage of osmotic tension to assure adequate fill volume. Similarly, a container 100 fabricated with a hydrogel may have a slight osmotic tension adjustment effect. Further, drug delivery can be achieved by diffusion of the injected material from within the container to the surrounding tissues.

EXAMPLE 1

5 A container 100 was manufactured utilizing a commercially available 6 cm x 4 cm tissue expanding device available from Mentor Deutschland GmbH, catalog number 350-5301M. The tissue-expanding device includes a remote two-way injection port 102 attached to one end. The tissue-expanding device was cut in the longitudinal direction to a width of 2 cm. The upper and lower walls were temporarily sealed together along the cut lengths using cyanoacrylate glue and later permanently sealed using the silicon adhesive, below. This results in a container having a width of approximately 1.5 cm. A polypropylene mesh was placed on the container. A silicon adhesive (silicon monomer and a catalyst component) was brushed onto the mesh segment overlying the container and the underlying container and. After curing over night, the mesh was firmly attached to the container. The expandable container with external port was easily and reversible expandable. The manufactured container 100 provided the added bending stiffness along the area of its attachment to the mesh.

EXAMPLE 2

10 A configuration similar to Example 1 except that the injection port is incorporated as an integral part of one side of the expandable container. Container mounts to the mesh 12 by providing an opening 104 in the mesh 12 for the introduction of the injection port 102a as shown Figs. 4c-d.

15 Fig. 4e discloses a double walled self-sealing container 100 that eliminates the need for a separate injection port. Container 100 comprises an inner chamber 100c that preferably contains a centrally located plastic or metal barrier 105 to prevent needle penetration through the far wall while injecting the bulking agent. While injecting the bulking agent using, for example, a needle, puncture holes are created in the walls of the inner and outer chamber 100c, 100d, respectively. After removal of the injecting device, exact alignment of the inner and out chamber puncture holes is shifted. This shift results in effectively sealing the injection site.

Alternatively, a single walled self-sealing container may be used. The inner layer of such a container may have a soft plastically deformable coating. The coating acts to fill-in any injection puncture site resulting in sealing the container.

5 Tape 12 may be further modified to include a mechanical adjustment means to adjust the tape 12 after it has been implanted as discussed below. The mechanical adjustment means incorporate a suture 106 and 106a preferably located on either side of the central portion of the tape 12 as shown in Figs. 5a-c. Sutures 106 and 106a can be used in combination with a one-way suturing retaining device 108 as is disclosed in U.S. Patent No. 5,669,935, which is
10 incorporated in its entirety by reference herein. Retaining device is anchored to tape 12 using any biocompatible adhesive or attachment as is known to those skilled in the art. Another means includes a tie-wrap-type mechanism to adjust the length of one or both sides of the tape 12 in near proximity to the urethra 54 and similarly positioned as sutures 106, 106a. In either instance, the sutures 106, 106a or tie wrap remain accessible through the incision in the vagina, discussed
15 below, for a period of time after tape implantation. Tape adjustment would be suitable for a number of days following the procedure before serious tissue ingrowth occurs. Afterward, the exposed sutures or tie-wrap may be cut.

20 In one embodiment tape 12 may be attached to needle segment 20 by means of tying, gluing or other suitable attaching means. Preferably, a bio-compatible heat shrink tube fixes tape 12 onto needle portion 20, Fig. 2a. In a further embodiment, as shown in Figs. 2b-d and 3a-h, needle 10 and tape 12 are further configured to enable easy attachment and detachment of tape 12 to and from needle 10 by the surgeon during the operation. This embodiment allows for the use
25 of a single needle for the procedure. This embodiment also allows for the use of a tape constructed, at least in part, of natural materials, which are otherwise not suitable in the pre-affixed embodiment due to the inability of the natural material to survive extended periods in inventory.

30 In one embodiment, shown in Figs. 3a-c, shaft 18 provides for a notch or slot 40 to slidably receive connecting tabs 32 and 32a that are attached at either ends of

tape 12 (Figs. 2b-d). Preferably, slot 40 extends through curved shaft 18 and is further located at the distal end 17 of needle 10 so that tape 12 may be disconnected from needle 10 immediately after needle 10 penetrates the abdomen wall, discussed below.

5 Tab 32 may be constructed from any bio-compatible material, such as plastic or metal. Tab 32 can be any shape, such as a square or arrow shape, so long as tap 32 can be securely inserted into notch or slot 40. Fig. 3b-c illustrates tab 32 having two spring arms 33 and 33a that when inserted into slot 40 expand and securely fasten tab 32 within slot 40. Tab 32 may be attached to tape 12 in any
10 number of convenient methods as previously discussed and well known to those skilled in the art.

Fig. 3d-e illustrates a two-tier slot 40, wherein tab 32 and spring element 33b slide into the lower tier which holds tab 32 in place. Alternate means of capturing tab 32 within slot 40 are available as is well known in the art.

15 Figs. 3f-g illustrate an alternate embodiment of affixing tape 12 to the distal end 17a of needle 10. A detachable blunt tip 16d having a connecting post 15, attaches to the distal end 17a by means of a mounting hole 15a to accept post 15. Post 15 may be securely attached to hole 15a either by compression fit, mating threads or other convenient attachment methods. Distal end 17a further defines a
20 groove 23 of varying depth to allow the end of tape 12 connected to post 15 to transition from within hole 15a to the exterior of needle 10. Along with the embodiment of Figs. 3a-e, this embodiment allows the surgeon to affix tape 12 to needle 10 just prior to the surgical procedure. One advantage is the ability to use a tape 12 constructed of, at least in part, a natural material 13.

25 As would be appreciated by one skilled in the art, there exist multiple means for detachably connecting the tape to the needle. Alternate embodiments would include tying the ends of tape 12 to form a knot and securely inserting the knot into a V-type groove in shaft 18. Alternately, a diagonal slit in shaft 18 could accept tape 12 or a suture extending from tape 12.

5 The surgical procedure for implanting tape 12 using two needles is shown in Figs. 6a-h utilizing the needle embodiment illustrated in Figs. 1 and 2a. In the figures the relevant parts of the female lower abdomen are disclosed, the vagina being 50, the uterus 52, the urethra 54, the pubic bone 56, the urinary bladder 58 and the abdominal wall 60. The first needle 10a penetrates the vaginal wall, an incision having first been made in the wall to create a tissue flap. The needle is attached to handle 411, and, the surgeon guides needle 10a through the vaginal wall and through the soft tissue on one side of the urethra 54, the needle then according to Fig. 6b being passed close to the back of the pubic bone 56, through additional layers of fat, muscle and fascia, and then through the abdominal wall 60 above the pubic bone 56. An incision can be made through the abdominal wall for the passage of the needle therethrough. The handle 411 is disconnected from needle 10a, Fig. 6c, and the needle 10a along with tape 12 are withdrawn from the abdomen wall by means of forceps, Fig. 6d.

10 Referring to Fig. 6e, needle 10b is now attached to handle 411. The surgeon passes needle 10b through the incision in the vaginal wall and through the soft tissue, again, on the opposite side of the urethra than the previous end of tape 12. Needle 10b passes close to the back of the pubic bone, through additional layers of fat, muscle and fascia, Fig. 6f, and then through the abdominal wall above the pubic bone and withdrawn, Fig. 6g.

15 Figs. 7a-g illustrate an alternate method of implanting tape 12 using a single needle 10. Tape 12 is attached to needle 10 by means of spring tab 32 as shown in Figs. 3b-c. Needle 10 penetrates the vaginal wall, an incision having first been made in the wall to create a tissue flap. The surgeon guides needle 10 through the vaginal wall and through the soft tissue on one side of the urethra 54, the needle then according to Fig. 7b being passed close to the back of the pubic bone 56, through additional layers of fat, muscle and fascia, and then through the abdominal wall 60 above the pubic bone 56. An incision can be made through the abdominal wall for the passage of the distal end 17 therethrough. Needle 10 only continues to pass through the abdominal wall until tap 32 may be disconnected from needle 10,

Fig. 7c. To do so, the surgeon simply pushes tab 32 through slot 40 using an appropriate instrument and cuts tab 32 pulls out tab 32 using forceps. Tab 32 may then be cut off and tape 12 may be pulled out of the abdominal wall to allow the surgeon additional length for the procedure. Needle 10 is then removed from the patient along the same path that it entered, but in the opposite direction, Fig. 7d. Alternatively, needle 10 may be disconnected from handle 411 and pulled out through the abdomen wall 60 using forceps as discussed with regard to the two needle procedure.

Needle 10 is now attached to the opposite end of tape 12 using connector tab 32a. The surgeon passes needle 10 through the incision in the vaginal wall and through the soft tissue on the opposite side of the urethra than the previous end of tape 12, Fig. 7e. Needle 10 passes close to the back of the pubic bone, through additional layers of fat, muscle and fascia, Fig. 7f, and then through the abdominal wall above the pubic bone. Needle 10 continues to pass through the abdominal wall only until tab 32a may be disconnected from needle 10, Fig. 7g. Tape 12 may be pulled out of the abdominal wall to allow the surgeon additional length for the procedure. Needle 10 is then removed from the patient along the same path that it entered, but in the opposite direction. Alternatively, needle 10 may be disconnected from handle 411 and pulled out through the abdomen wall 60 using forceps.

Since both procedures may be performed using a local anesthesia, the patient is able to provide feedback to the surgeon after tape 12 is in place. Typically, the urinary bladder 58 is filled with a fluid, such as water, using a catheter and the patient is requested to cough. The surgeon is able to determine the operation of the urethra and may adjust the tape 12, as necessary, by adjusting the ends of tape 12 located at the outside of the abdomen 60, Figs. 6h and 7h. After adjustments, the surplus tape at the abdomen is cut off, and the ends of the tape are secured within the abdomen and the abdomen is closed. Likewise, the incision at the vaginal wall is closed whereby the tissue flap seals the tape between the urethra 54 and the wall of vagina 50.

Tape 12 is left in the body and forms an artificial ligament attached to the abdominal wall that provides the support for the urethra as required in order to restore urinary continence to the patient.

At the end of either procedure disclosed in Figs. 6 and 7, the surgeon may perform a test procedure to determine the integrity of the urinary bladder. A hydraulic diagnosis of the bladder may be performed by placing a rigid endoscope/sheath transurethrally and injecting fluid through the sheath into the bladder. The bladder is pressurized to a known level, about 50 mm Hg as measured through the sheath. If the pressure is maintained, then the surgeon can be confident that the bladder has not been perforated. Conversely, if the bladder loses pressure, steps can be taken to repair any defects.

Post-surgical adjustment of the tape may be accomplished by injecting bulking agents in the vicinity of the tape sling so as to effect additional support to the urethra. Preferably the bulking agent would be injected at the top of the mesh so as to expand the tissue between mesh and urethra (direct bulking) as shown in Figure 8. This procedure may be used in combination with a tape 12 having an expandable chamber or used alone. Suitable direct bulking agents include DURASPHERES, CONTIGEN, MACROPLASTIQUE as well as polytetrafluorethylene, and synthetic, natural slowly absorbable or nonabsorbable materials. Bulking agents must be stable, biocompatible and, in the case of direct injection without a container, should be resistant to migration. The bulking agent may be detectable (eg., radiopaque) such as the case with DURASPHERES or may contain a contrast component that allows for visualization of the amount and location of the agent.

To inject a bulking agent into container 100 (Figs. 4a-f), the surgeon would palpate the area to detect the injection site for the container, and if needed, a small incision in the vaginal wall may be made. Alternatively, markers may be either separate or an integral part of the container or tape. For example, ultrasound may be used to provide guided injection. This may be achieved

preferably by rectal placement of the transducer. A suitable bulking agent may then be injected using only local anesthesia, transvaginally or transurethrally.

The ultrasonic diagnostic detectability of the targeting region could be improved by radiopaque beads if desired. Referring to Fig. 9, an x-ray detectable polypropylene (for example, Prolene, provided by Ethicon, Inc.) foil ring 109 may be used. An exemplary ring 109 has an inner diameter of 0.5 cm and an outer diameter of 1 cm and a thickness of 0.5 mm and contains six 1.5 mm diameter zirconiumdioxide beads (95% ZrO_2 / 5% Y_2O_3 provided by Mühlmeier Mahlechnik, Germany) as radiopacifiers around an opening in the mesh 12. Ring 109 is affixed to the center of tape 12 using ultrasonic welding. These x-ray radiopacifiers are suitable implant materials and are also visible in ultrasound.

Ring 109 may also be used for x-ray-guided injection. After tape implantation, the area around the tape may be expanded with a bulking agent using guidance provided by x-ray visualization. Exact positions of the target ring 109 and (and corresponding tape), radiopacified-filled urethra, bladder and bulking agent (for example, radiopaque DURASPHERES) may be determined through the use of computerized tomography.

It will be apparent from the foregoing that, while particular forms of the invention have been illustrated and described, various modifications can be made without departing from the spirit and scope of the invention. Accordingly, it is not intended that the invention be limited, except as by the appended claims.

CLAIMS

We Claim:

1. A surgical instrument for treating female urinary stress incontinence comprising:
 - a) a tape for implanting into the lower abdomen of a female to provide support to the urethra comprising adjusting means for adjusting the tape after implantation; and
 - b) a curved needle-like element defining in part a curved shaft having a distal end and a proximal end, and means for attaching to the tape.
2. The surgical instrument of claim 1 wherein the adjusting means is an expandable chamber.
3. The surgical instrument of claim 1 wherein the adjusting means is a suture-like element that passes through the tape, whereby when the suture element is tightened, the tape provides additional support to the urethra.
4. A surgical instrument for treating female urinary stress incontinence comprising a tape for implanting into the lower abdomen of a female to provide support to the urethra, the tape defining a first end and a second end and an expandable chamber for accepting a bulking agent.
5. A method for treating female urinary incontinence comprising the steps of:
 - a) providing a first and second curved needle-like element, each defining a curved shaft having a distal end and a proximal end, and a tape attached to both needle elements, the tape comprising an expandable container for receiving a bulking agent;

- b) passing the first needle and tape into the body via the vagina and on one side of the urethra and extending the tape over the pubic bone and through the abdomen wall;
- c) passing the second needle and tape into the body via the vagina and on the opposite side of the urethra than the first needle and extending the tape over the pubic bone and through the abdomen wall, creating a supporting sling below the urethra;
- d) leaving the tape implanted in the body; and
- e) injecting a bulking agent into the expandable container.

6. A method for treating female urinary incontinence comprising the steps of:
- a) providing a curved needle-like element defining in part a curved shaft having a distal end and a proximal end and a tape comprising attached thereto, the tape further comprising means for adjusting the tape; and
 - b) passing the needle and tape into the body via the vagina to form a sling around the urethra;
 - c) leaving the tape implanted in the body; and
 - d) adjusting the tape using the adjusting means.

7. A method for treating female urinary incontinence comprising the steps of:
- a) providing a curved needle-like element defining in part a curved shaft;
 - b) attaching a tape to the needle;
 - c) passing the needle and tape into the body;
 - d) attaching the tape to the needle and passing the needle and tape into the body to form a sling around the urethra;
 - e) leaving the tape implanted in the body; and
 - f) adjusting the tape after implantation.

8. A method for treating female urinary incontinence comprising the steps of:

- g) providing a curved needle-like element defining in part a curved shaft;
- h) attaching a tape to the needle;
- i) passing the needle and tape into the body;
- j) attaching the tape to the needle and passing the needle and tape into the body to form a sling around the urethra;
- k) leaving the tape implanted in the body; and
- l) injecting a bulking agent between the tape and urethra.

9. A device for supporting internal anatomical structure comprising a mesh tape and an expandable chamber having the ability to contain a variable amount of a bulking agent wherein the expandable chamber is affixed to the mesh tape and positioned between the mesh tape and anatomical structure.

ABSTRACT

**METHOD AND APPARATUS FOR ADJUSTING FLEXIBLE AREAL POLYMER
IMPLANTS**

A minimally invasive approach to adjusting the amount of support on an anatomical structure. The methods and apparatus described include the use of a tape for supporting an anatomical structure. Adjustment may be achieved by use of bulking agents applied either directly to the site or into a containment device located within proximity of the tape and such that it works in conjunction with the tape to support the anatomic structure. An alternative approach utilizes mechanical means for adjusting the effective length of the supporting arms of the tape used to support the anatomical structure.



FIG. 2a

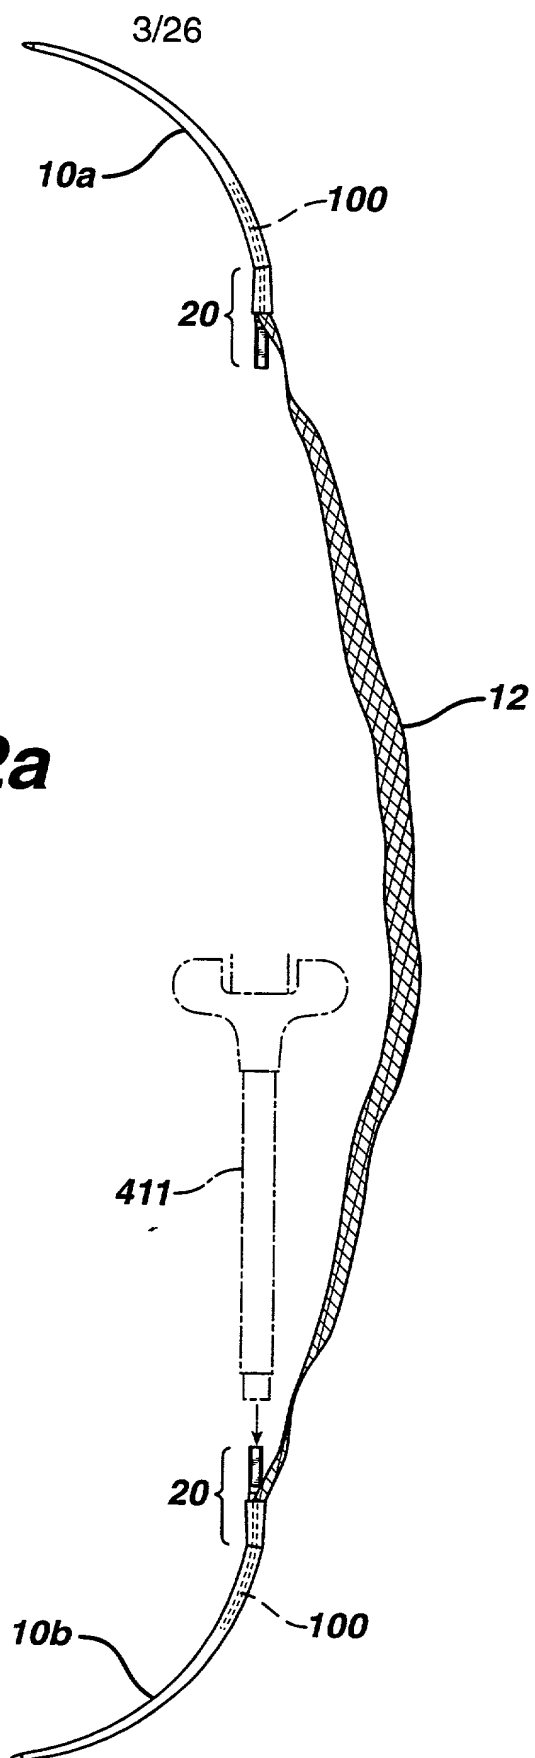


FIG. 2c



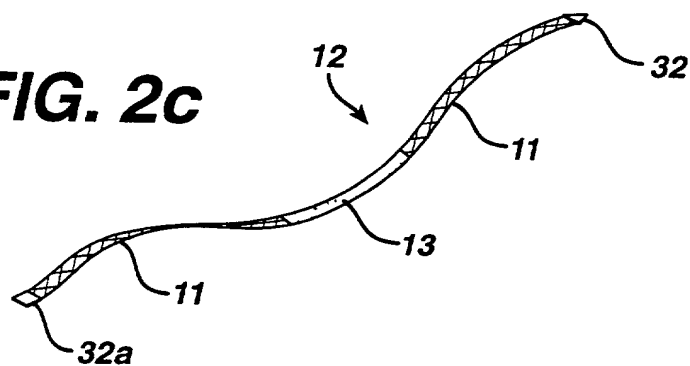


FIG. 2d

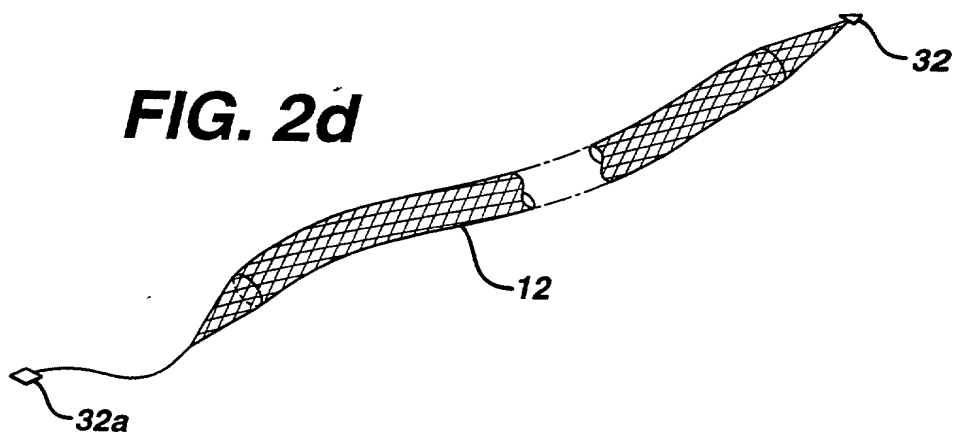

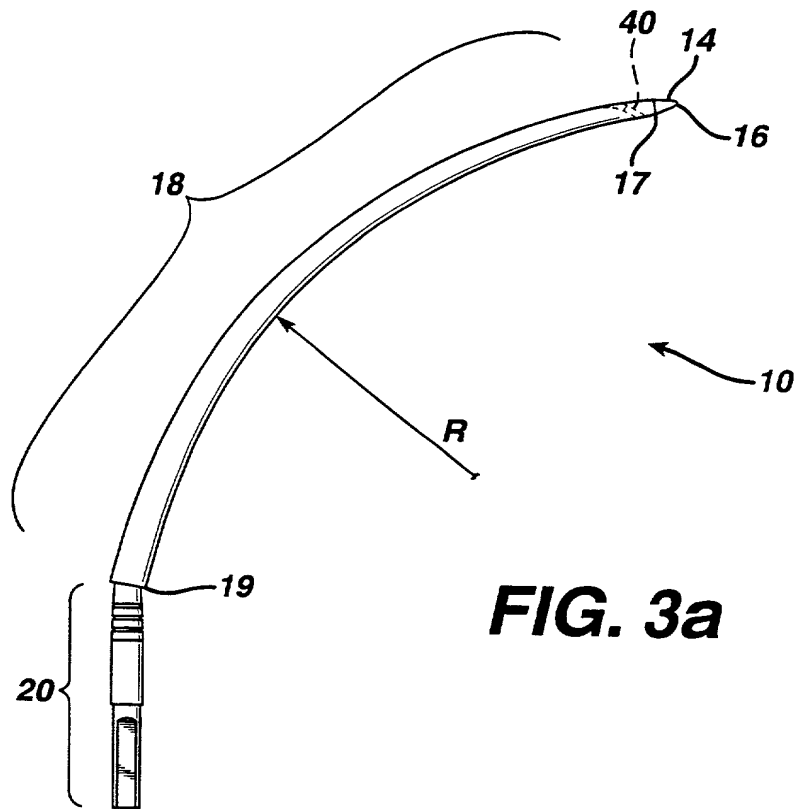

5/23

FIG. 3b

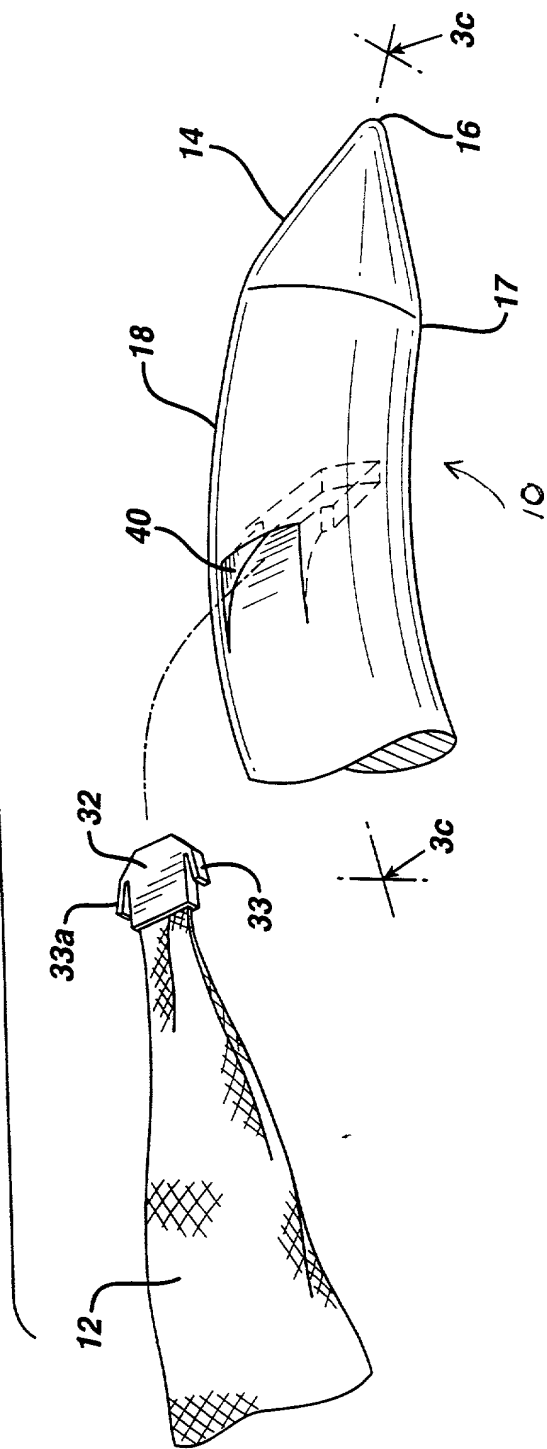


FIG. 3c

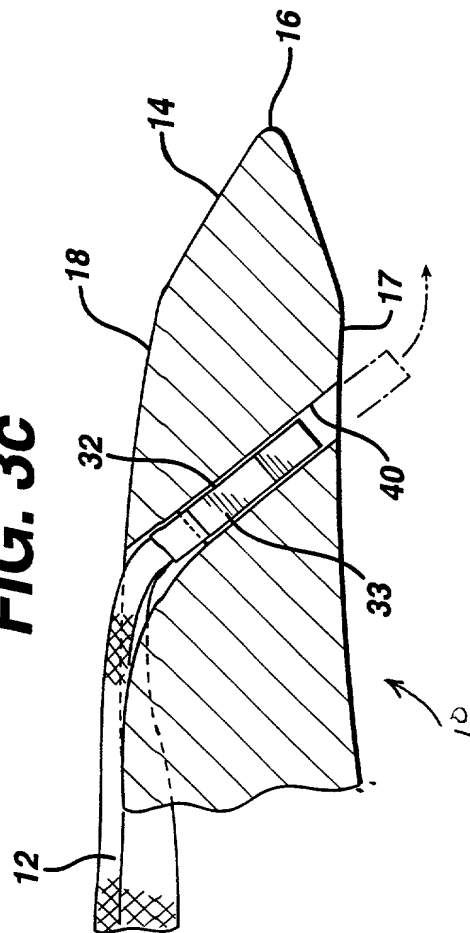


FIG. 3d

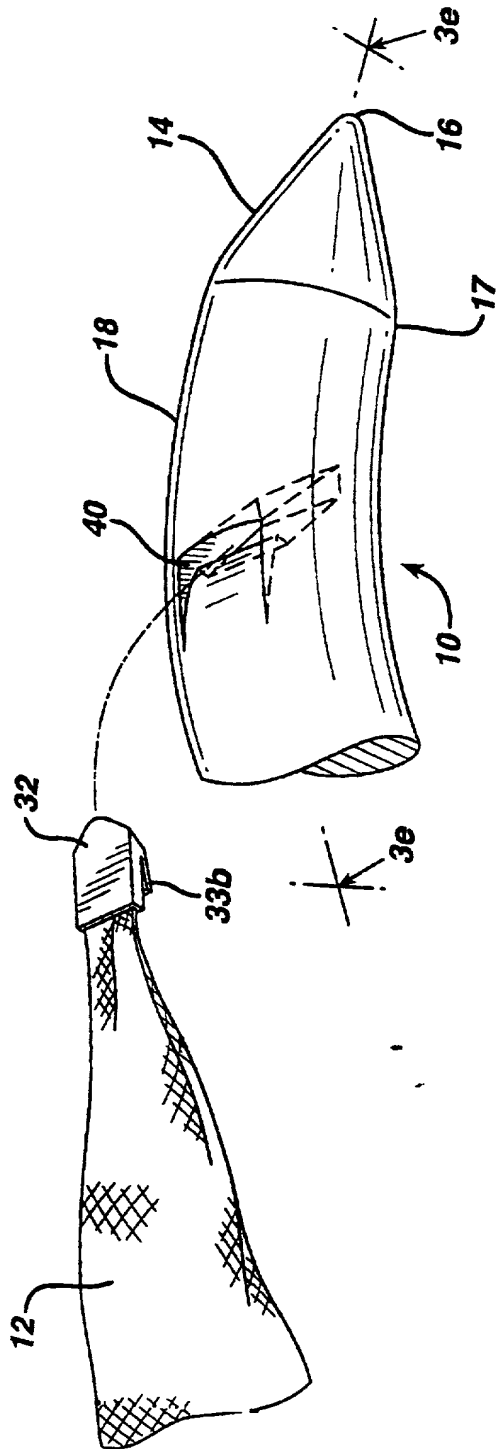
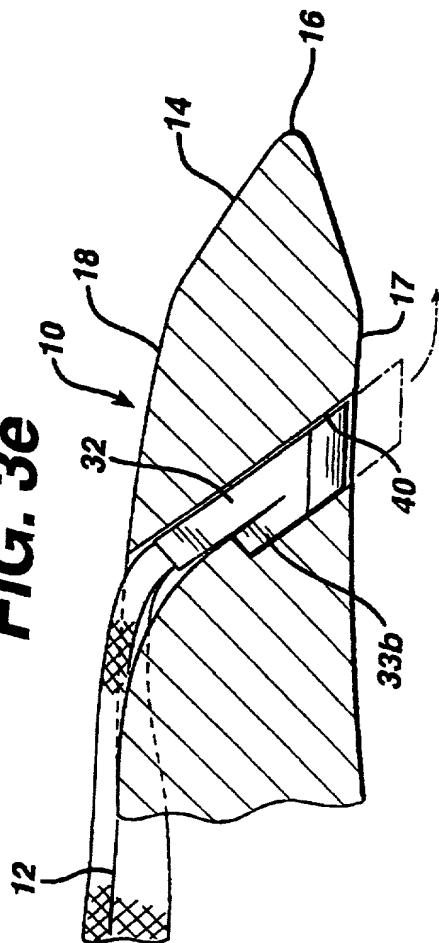
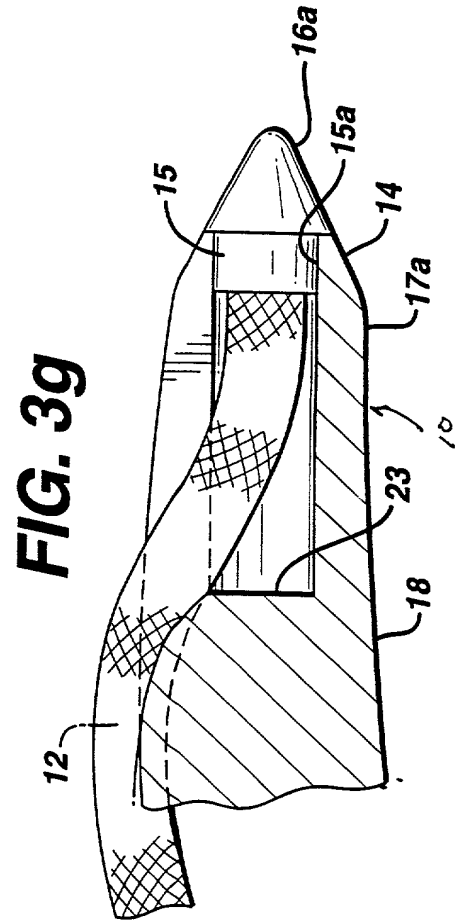
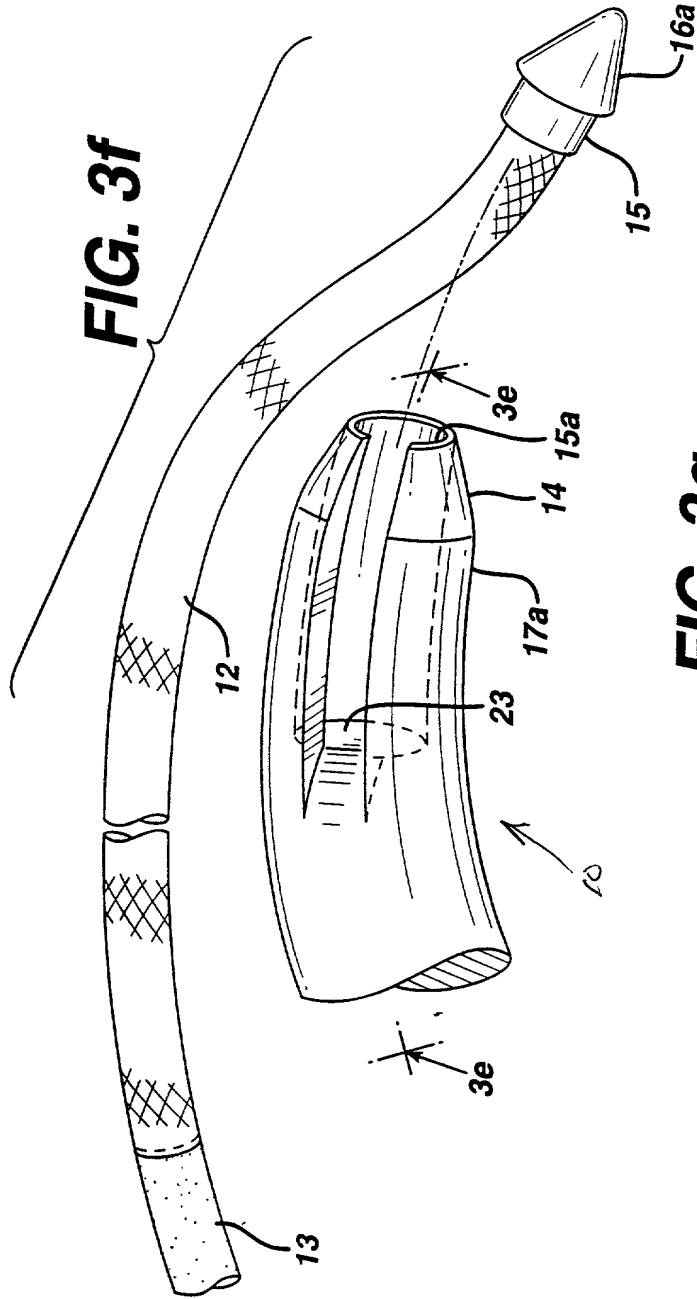


FIG. 3e





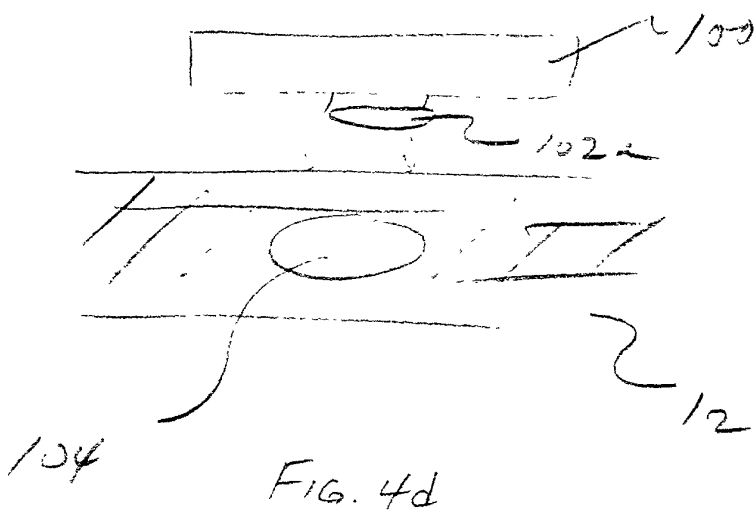


FIG. 4d

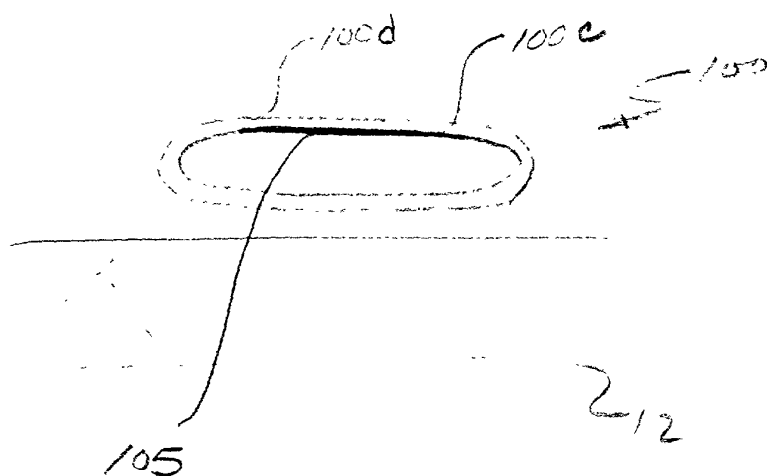


Fig 7e


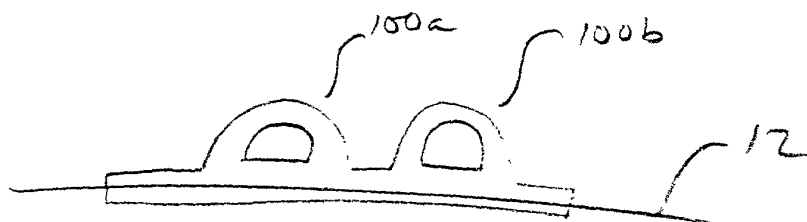


FIG. 4 f

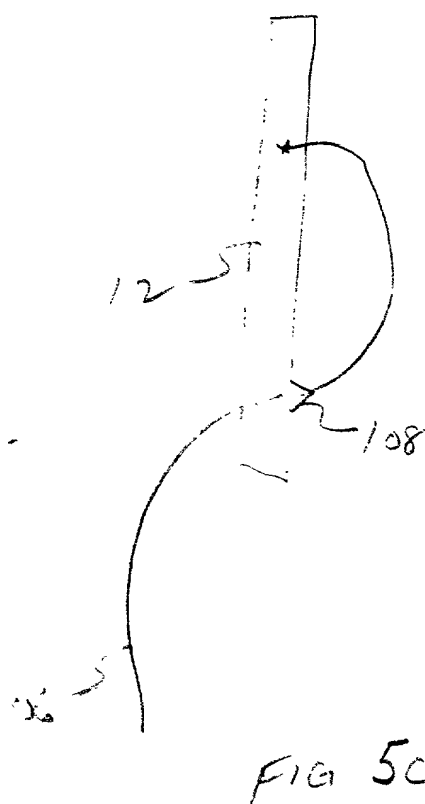

The 1990s		The 2000s	
Year	Country	Year	Country
1990	USA	2000	USA
1991	USA	2001	USA
1992	USA	2002	USA
1993	USA	2003	USA
1994	USA	2004	USA
1995	USA	2005	USA
1996	USA	2006	USA
1997	USA	2007	USA
1998	USA	2008	USA
1999	USA	2009	USA
2000	USA	2010	USA
2001	USA	2011	USA
2002	USA	2012	USA
2003	USA	2013	USA
2004	USA	2014	USA
2005	USA	2015	USA
2006	USA	2016	USA
2007	USA	2017	USA
2008	USA	2018	USA
2009	USA	2019	USA
2010	USA	2020	USA
2011	USA	2021	USA
2012	USA	2022	USA
2013	USA	2023	USA
2014	USA	2024	USA
2015	USA	2025	USA
2016	USA	2026	USA
2017	USA	2027	USA
2018	USA	2028	USA
2019	USA	2029	USA
2020	USA	2030	USA
2021	USA	2031	USA
2022	USA	2032	USA
2023	USA	2033	USA
2024	USA	2034	USA
2025	USA	2035	USA
2026	USA	2036	USA
2027	USA	2037	USA
2028	USA	2038	USA
2029	USA	2039	USA
2030	USA	2040	USA
2031	USA	2041	USA
2032	USA	2042	USA
2033	USA	2043	USA
2034	USA	2044	USA
2035	USA	2045	USA
2036	USA	2046	USA
2037	USA	2047	USA
2038	USA	2048	USA
2039	USA	2049	USA
2040	USA	2050	USA
2041	USA	2051	USA
2042	USA	2052	USA
2043	USA	2053	USA
2044	USA	2054	USA
2045	USA	2055	USA
2046	USA	2056	USA
2047	USA	2057	USA
2048	USA	2058	USA
2049	USA	2059	USA
2050	USA	2060	USA
2051	USA	2061	USA
2052	USA	2062	USA
2053	USA	2063	USA
2054	USA	2064	USA
2055	USA	2065	USA
2056	USA	2066	USA
2057	USA	2067	USA
2058	USA	2068	USA
2059	USA	2069	USA
2060	USA	2070	USA
2061	USA	2071	USA
2062	USA	2072	USA
2063	USA	2073	USA
2064	USA	2074	USA
2065	USA	2075	USA
2066	USA	2076	USA
2067	USA	2077	USA
2068	USA	2078	USA
2069	USA	2079	USA
2070	USA	2080	USA
2071	USA	2081	USA
2072	USA	2082	USA
2073	USA	2083	USA
2074	USA	2084	USA
2075	USA	2085	USA
2076	USA	2086	USA
2077	USA	2087	USA
2078	USA	2088	USA
2079	USA	2089	USA
2080	USA	2090	USA
2081	USA	2091	USA
2082	USA	2092	USA
2083	USA	2093	USA
2084	USA	2094	USA
2085	USA	2095	USA
2086	USA	2096	USA
2087	USA	2097	

FIG. 6a



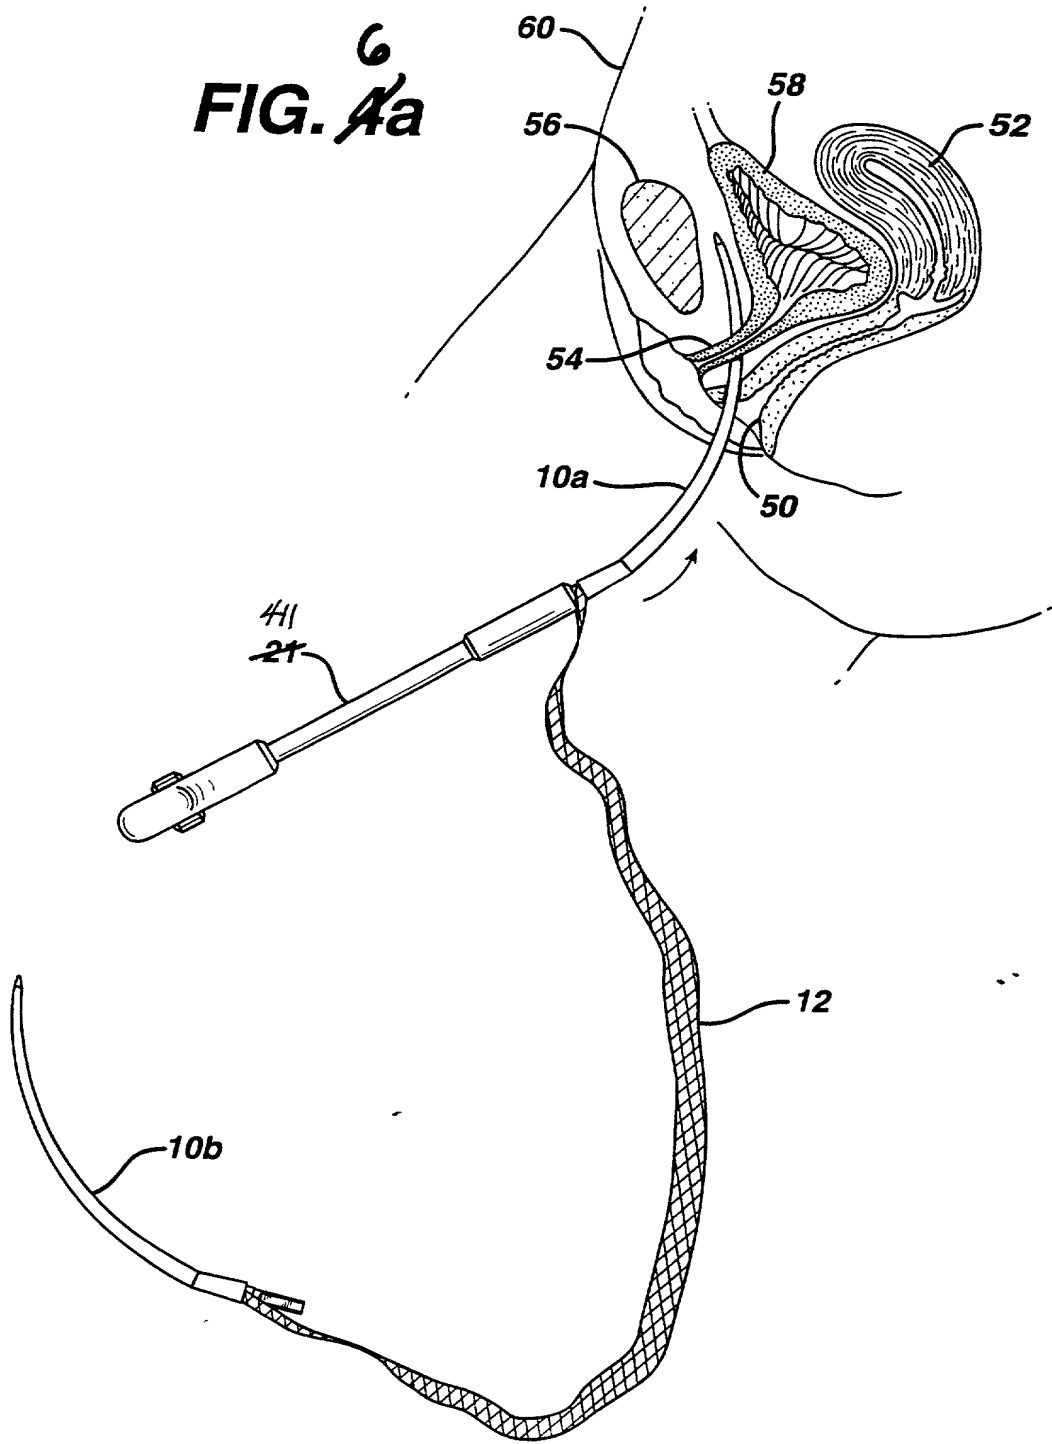


FIG. 6
FIG. 4b

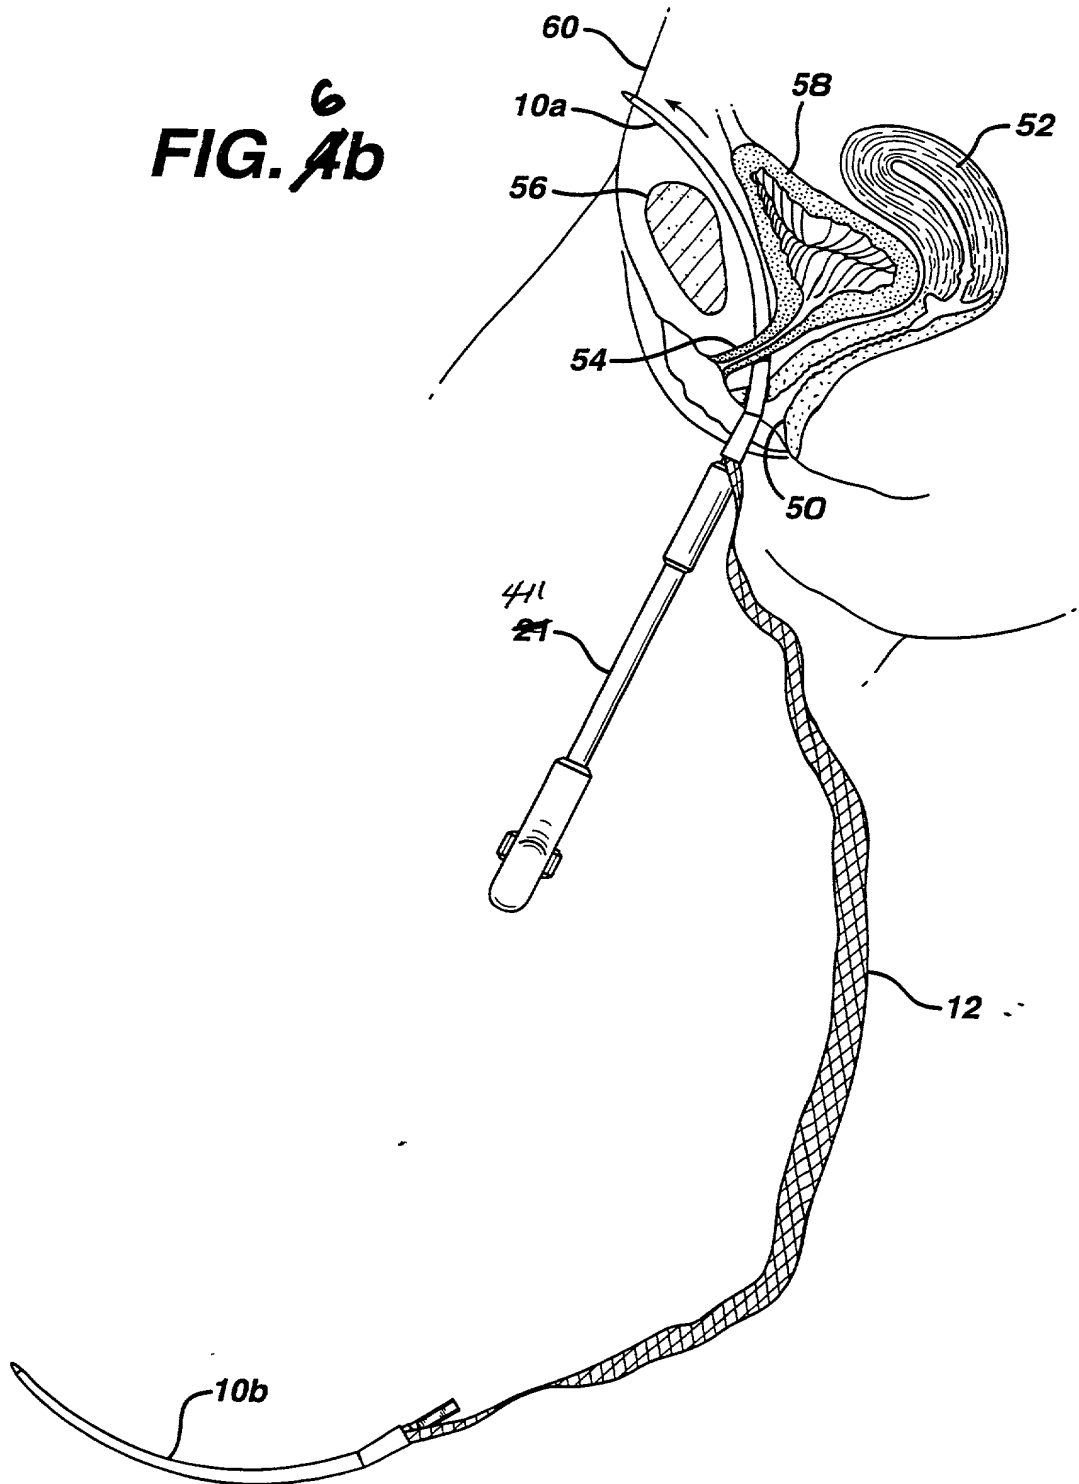

10/23


FIG. 6c

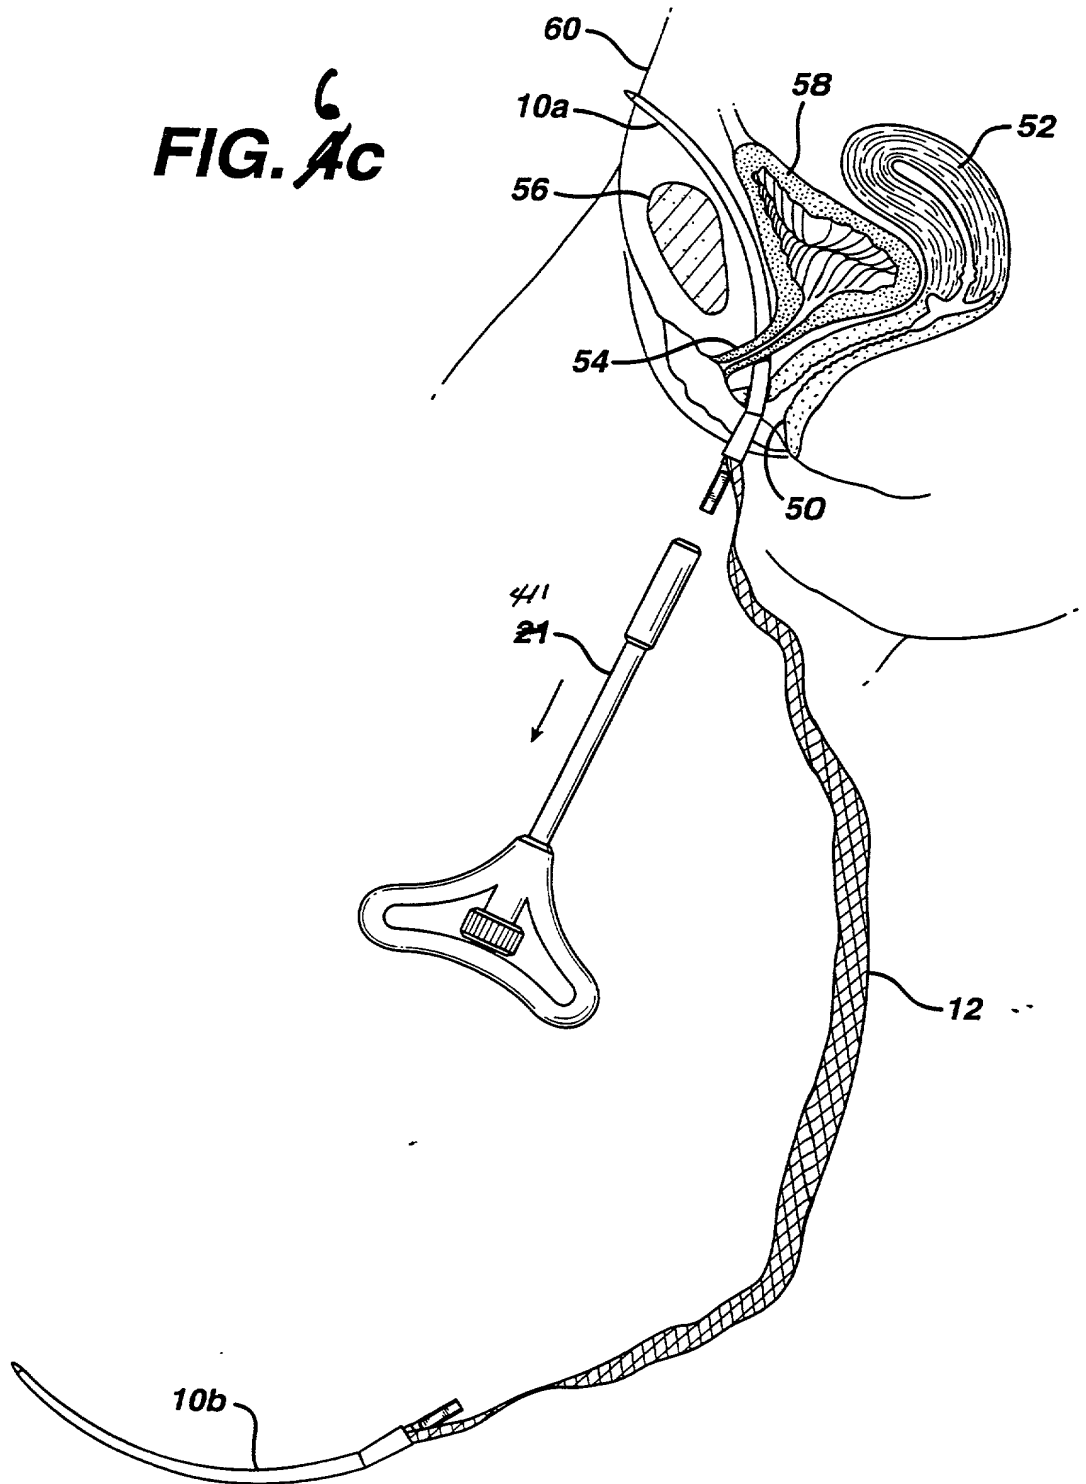

004090" 24263560

11/23


FIG. 4d

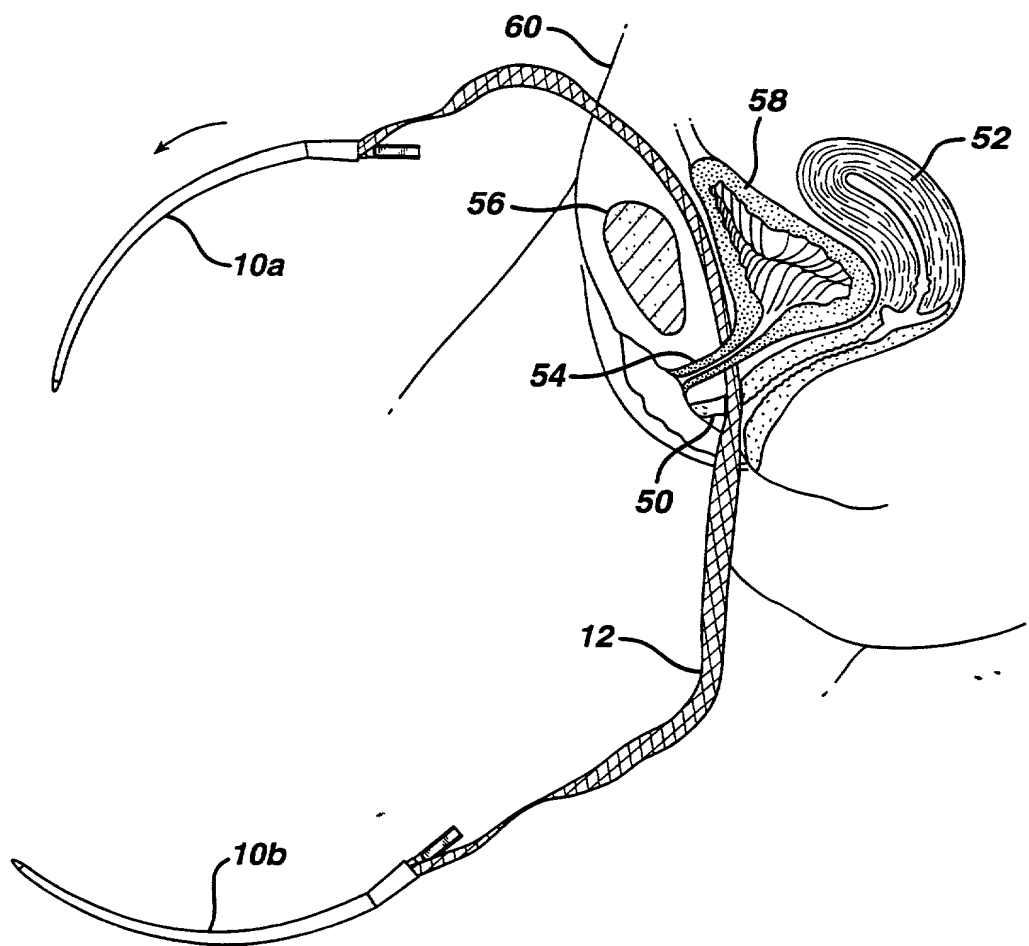

004090" 24268560


12/23

6
FIG. 4e

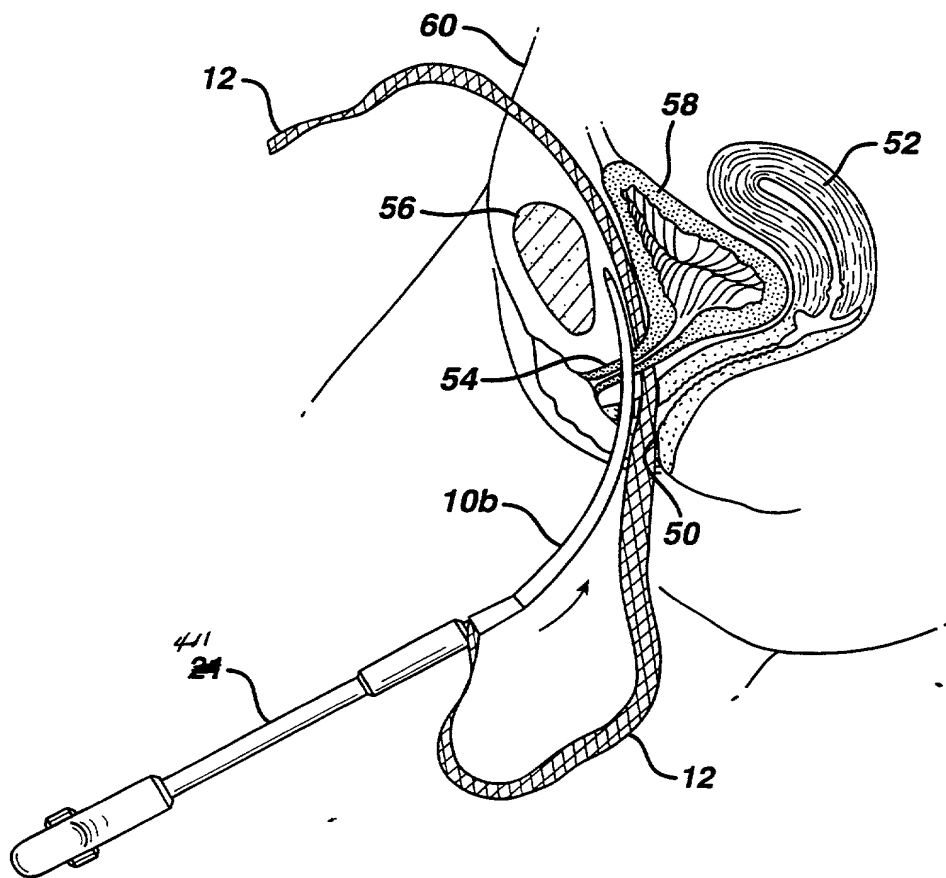


09589242-060700

⁶
FIG. Af

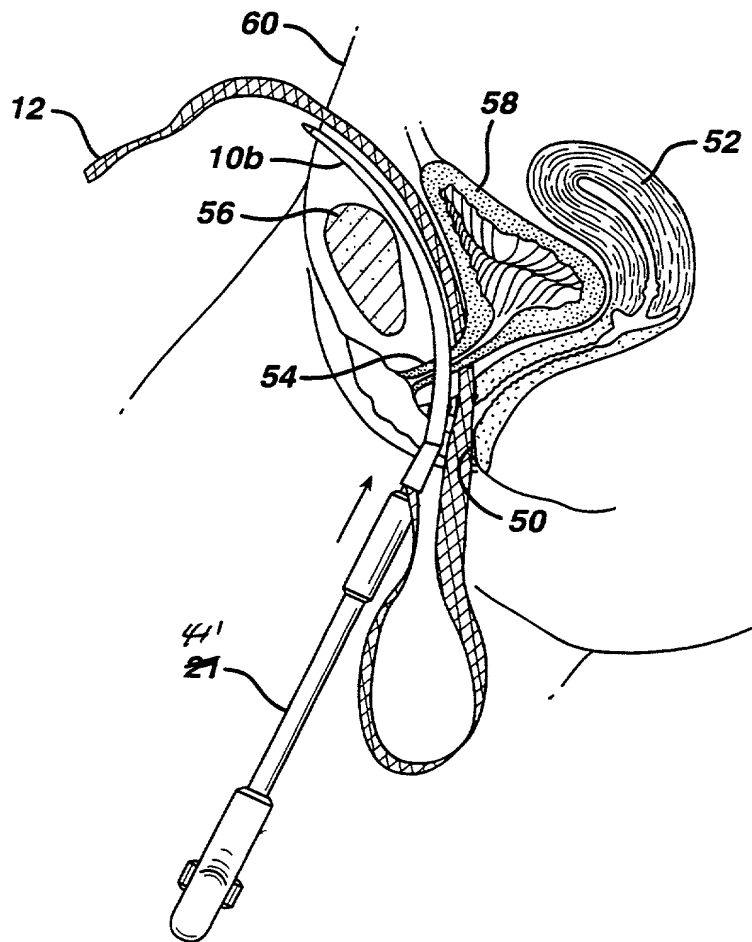

6.

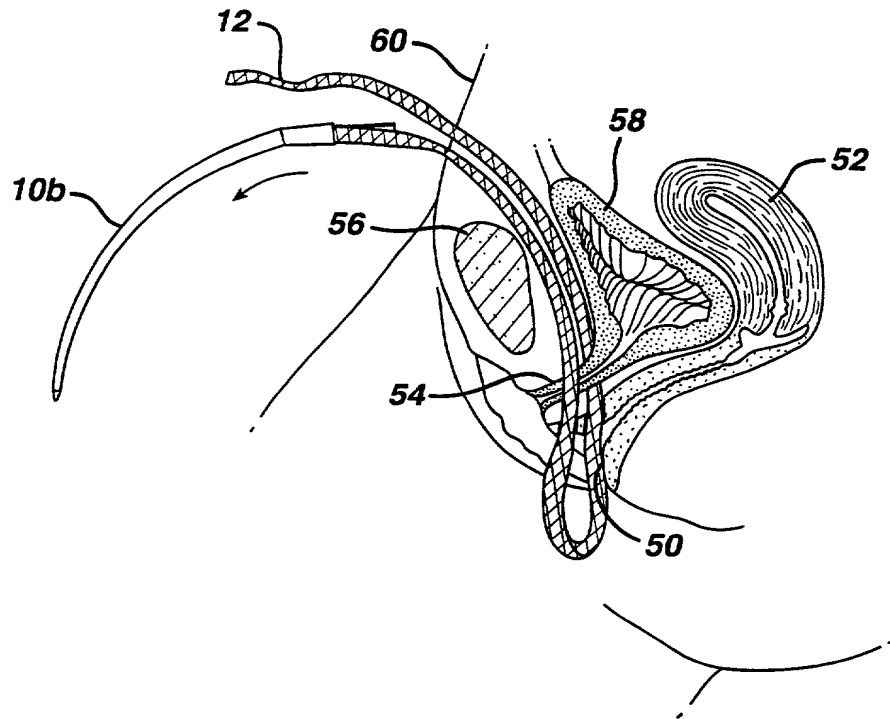

6

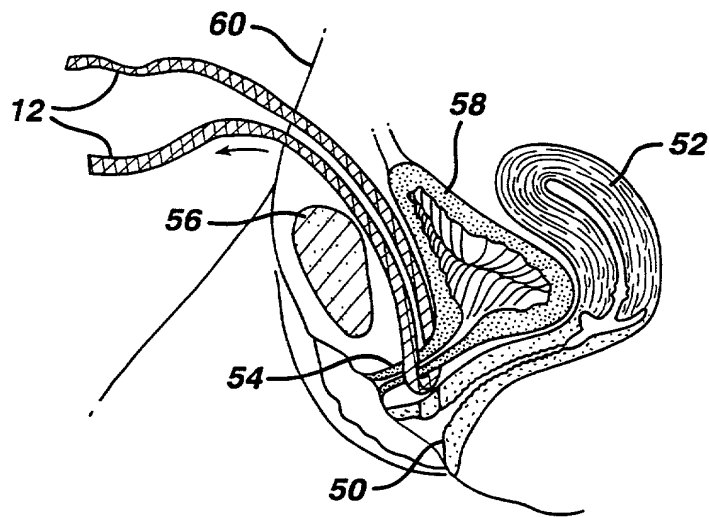


FIG. 3a

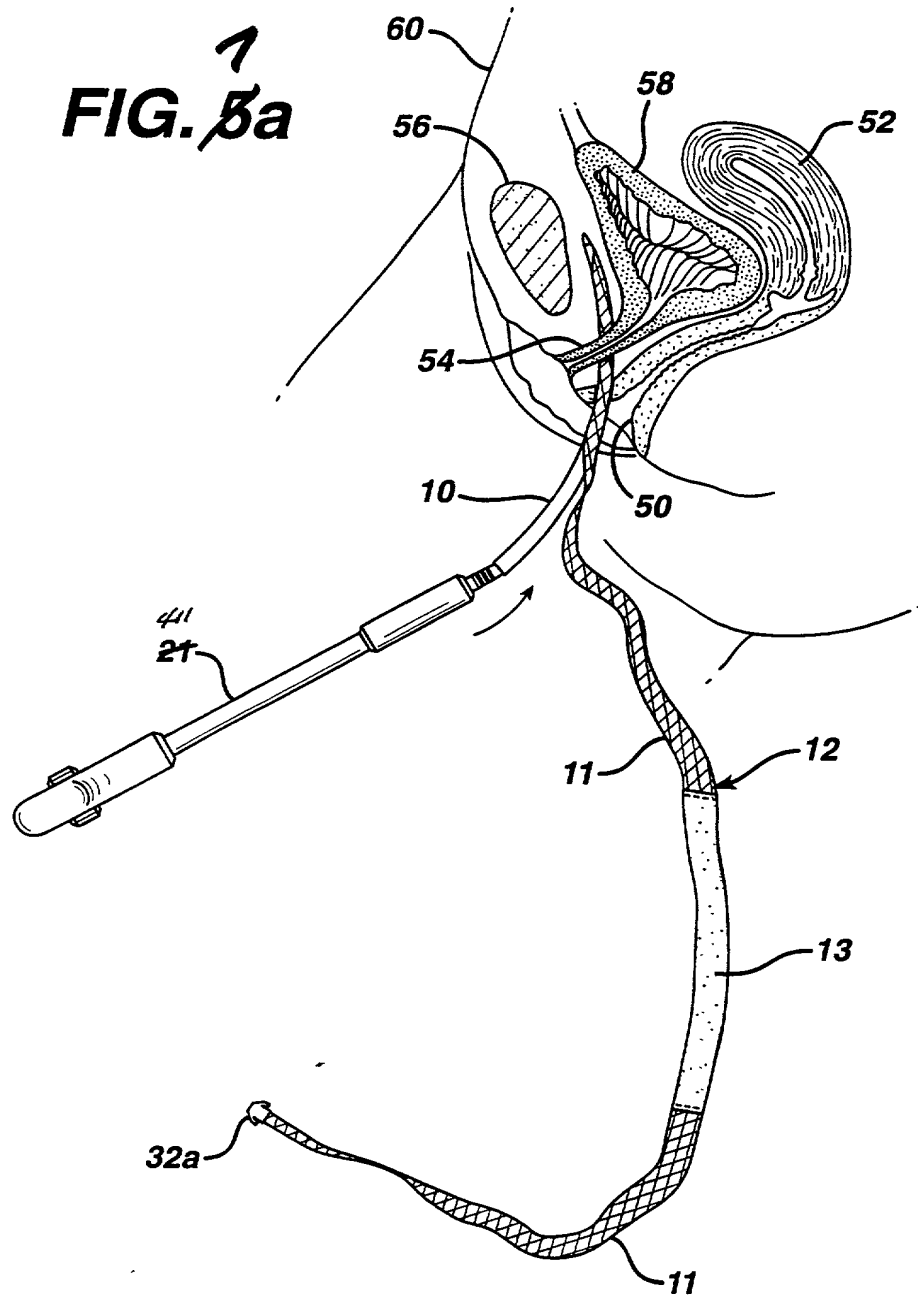


FIG. 5b


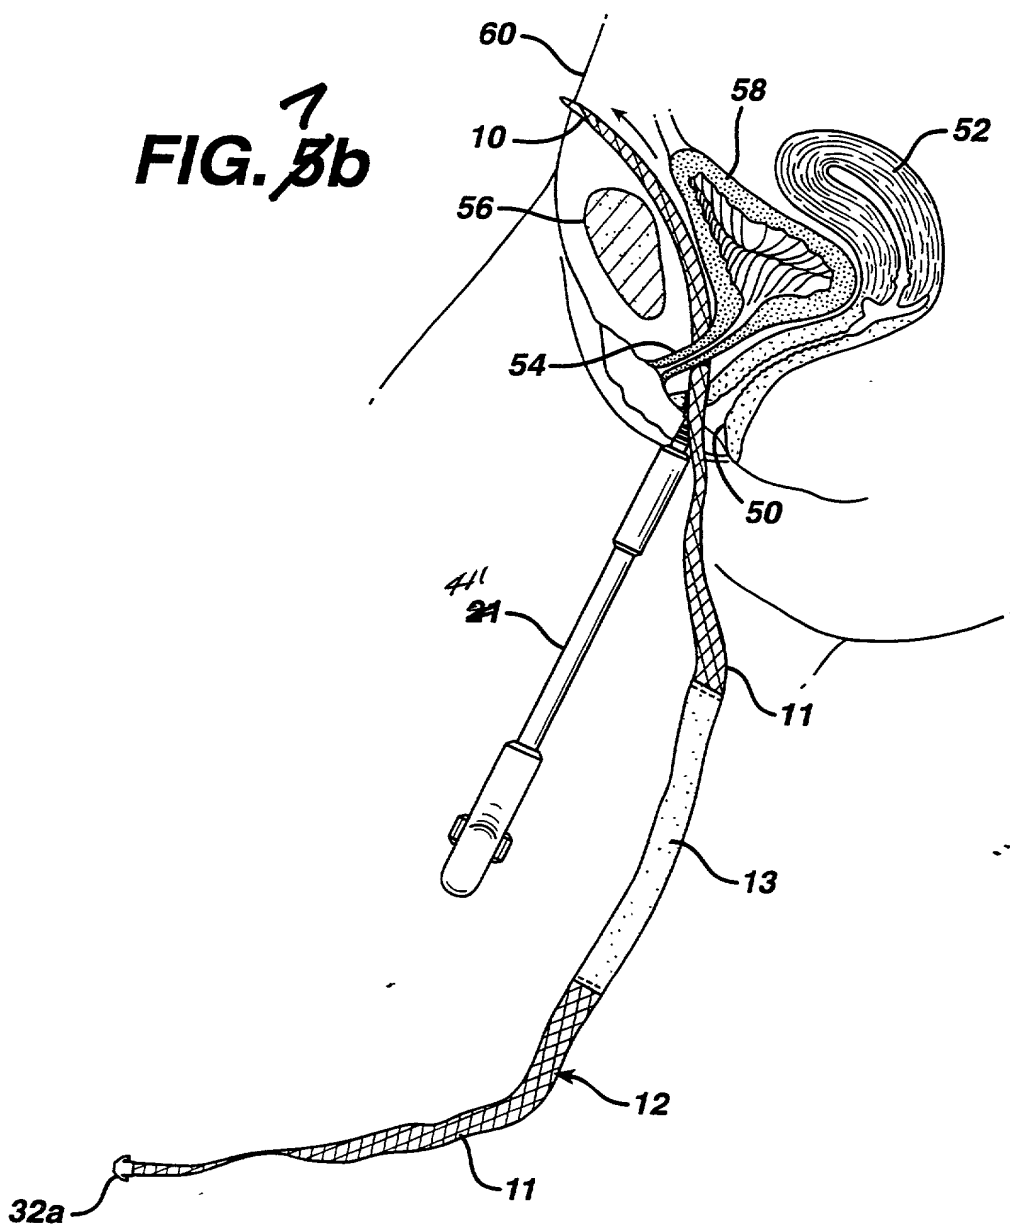


FIG. 3c

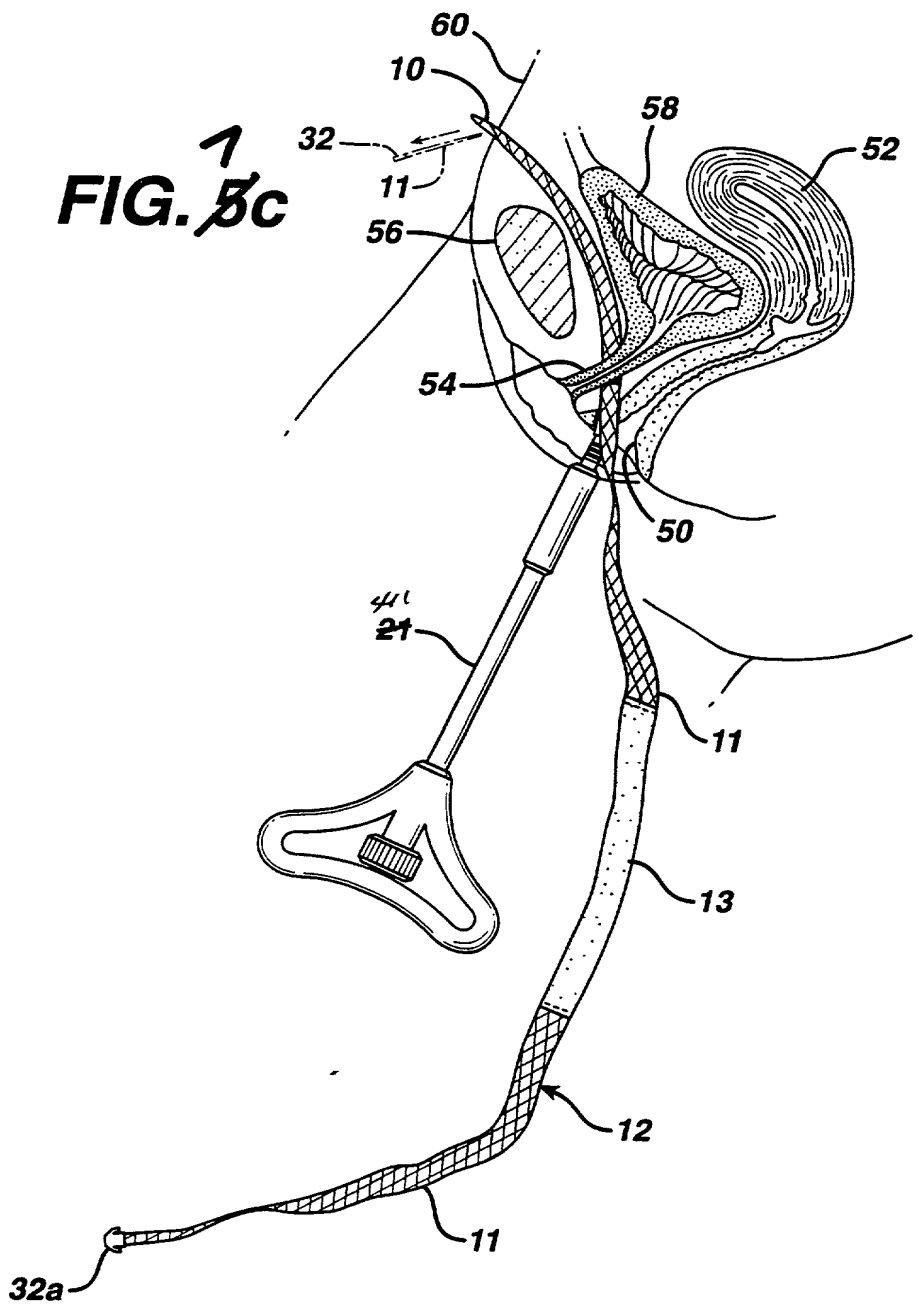

7

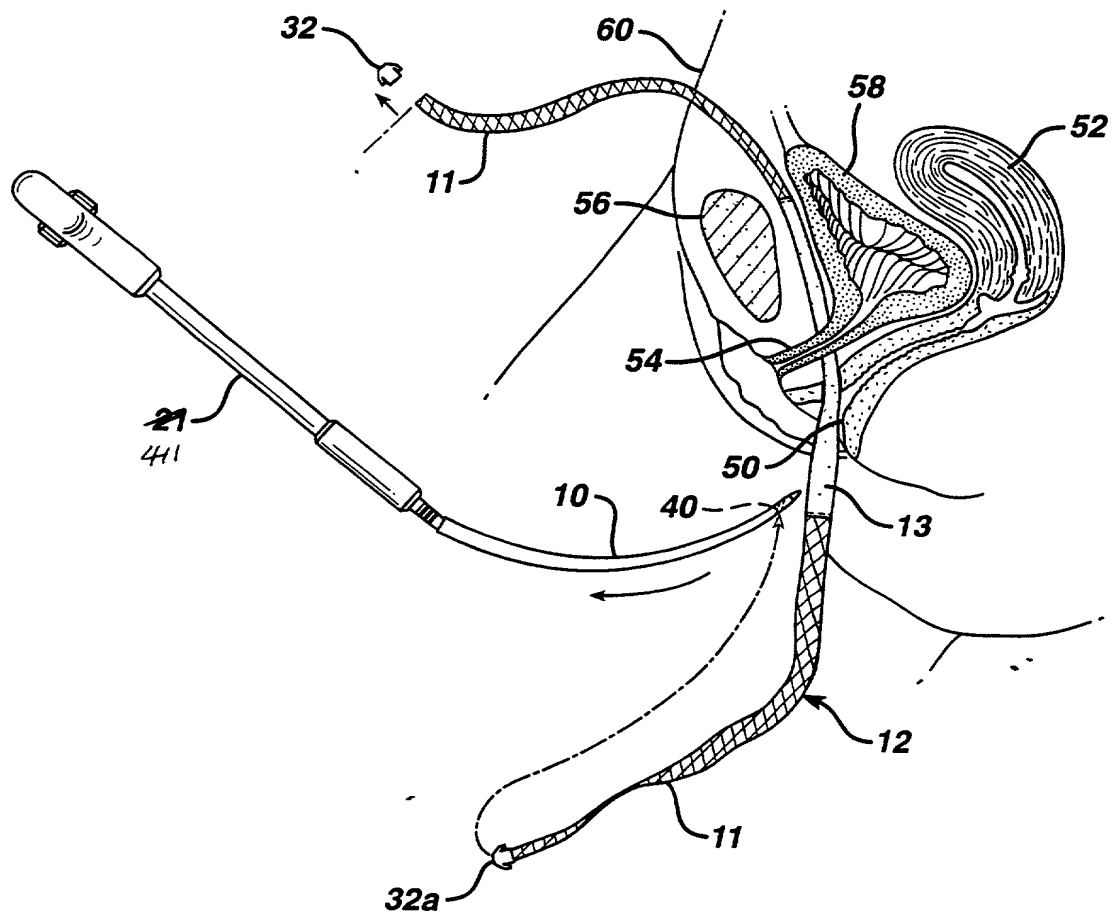


FIG. 1



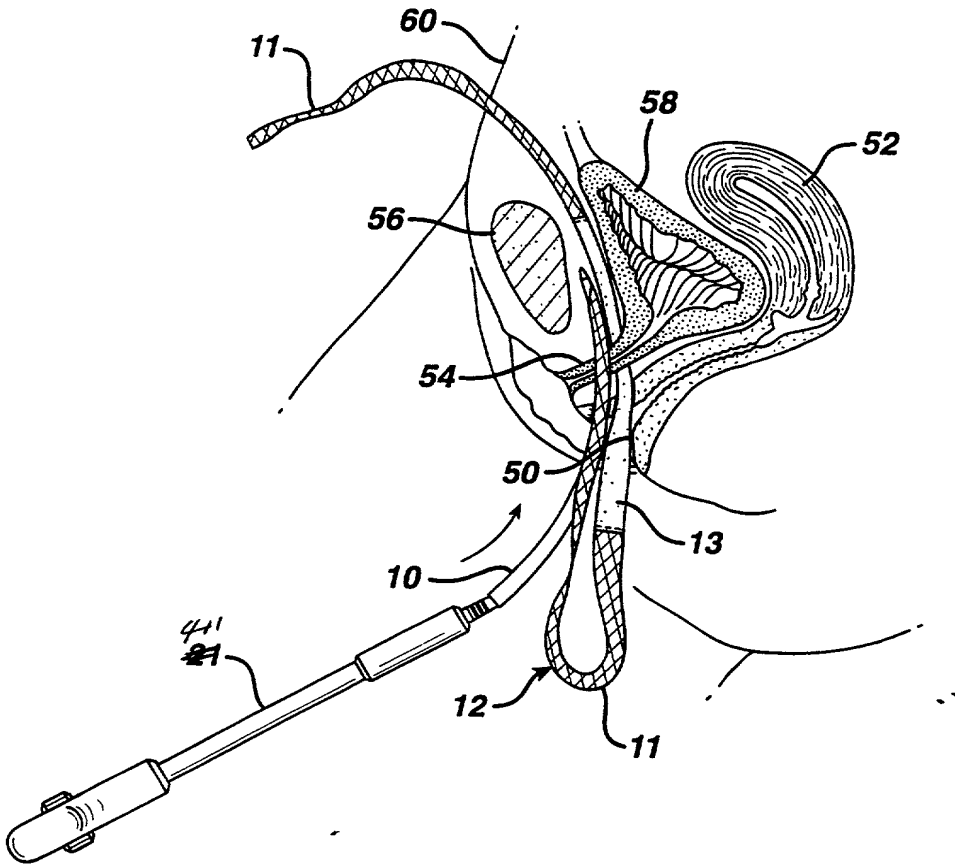


FIG. 1g

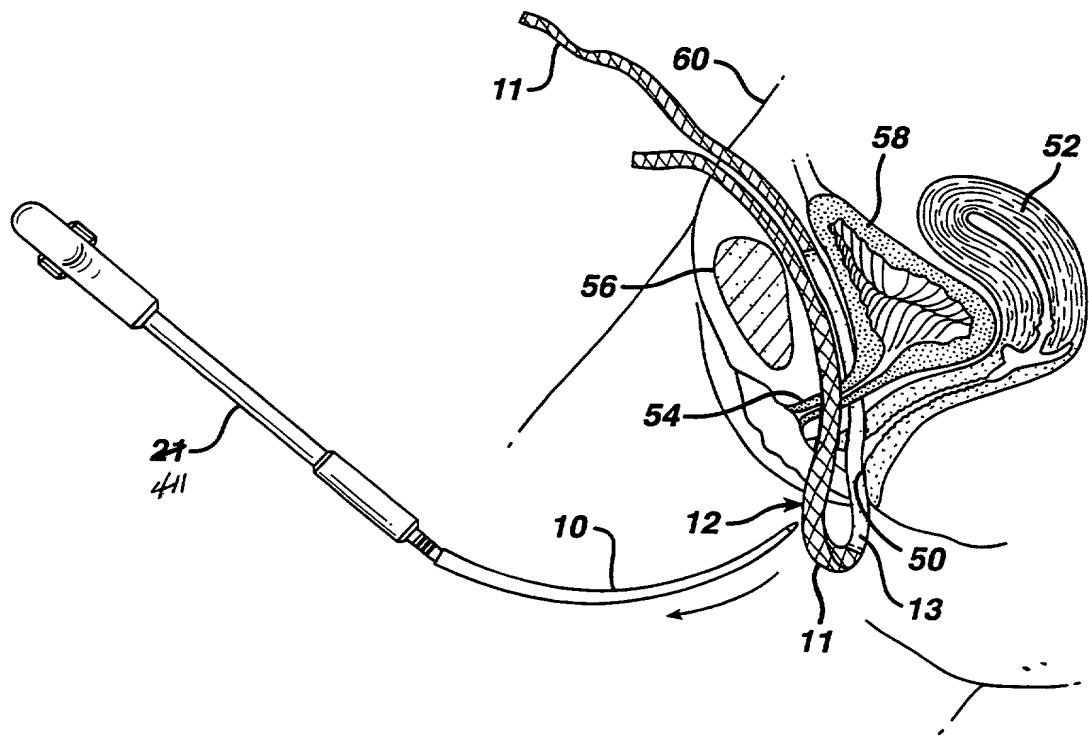

007090" 24268560

FIG. 5h

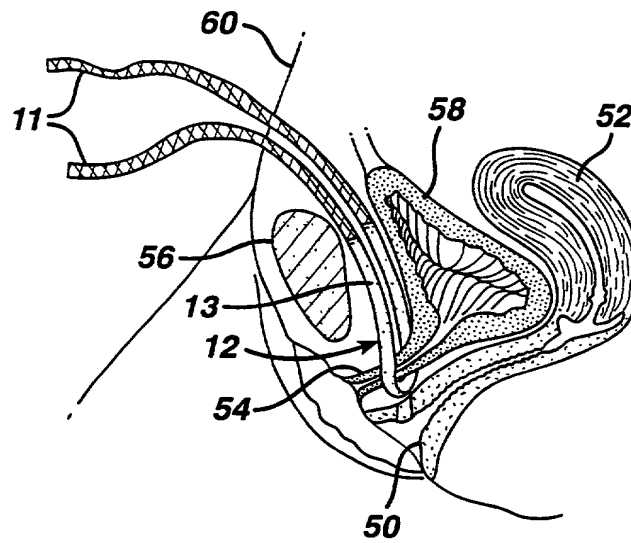

DECLARATION AND POWER OF ATTORNEY FOR PATENT APPLICATION

As a below named inventor, I hereby declare that:

My residence, post office address and citizenship are as stated below next to my name,

I believe I am the original, first and sole inventor (if only one name is listed below) or an original, first and joint inventor (if plural names are listed below) of the subject matter which is claimed and for which a patent is sought on the invention entitled METHOD AND APPARATUS FOR ADJUSTING FLEXIBLE AREAL POLYMER IMPLANTS, the specification of which

(check one) ☒ is attached hereto.

☐ was filed on _____ as

Application Serial No. _____

and was amended on _____.
(if applicable)

I hereby state that I have reviewed and understand the contents of the above-identified specification, including the claims, as amended by any amendment referred to above.

I acknowledge the duty to disclose information which is material to patentability as defined in 37 CFR 1.56.

I hereby claim foreign priority benefits under Title 35, United States Code, §119 (a)-(d) or §365(b) of any foreign application(s) for patent or inventor's certificate, or §365(a) of any PCT international application which designated at least one country other than the United States of America, listed below and have also identified below, by checking the box, any foreign application for patent or inventor's certificate, or of any PCT international application having a filing date before that of the application on which priority is claimed.

Prior Foreign Application(s):

Country	Application Number	Date of Filing	Priority Claimed Under 35 U.S.C. 119	
			<input type="checkbox"/> YES	<input type="checkbox"/> NO
			<input type="checkbox"/> YES	<input type="checkbox"/> NO
			<input type="checkbox"/> YES	<input type="checkbox"/> NO

I hereby claim the benefit under Title 35, United States Code, §119(e) of any United States provisional application(s) listed below:

60/138,231
(Application Number)

June 9, 1999
(Filing Date)

(Application Number)

(Filing Date)

I hereby claim the benefit under Title 35, United States Code, §120 of any United States application(s) listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35, United States Code, §112, I acknowledge the duty to disclose material information as defined in Title 37, Code of Federal Regulations, §1.56(a) which occurred between the filing date of the prior application and the national or PCT international filing date of this application:

Application Serial No. Filing Date Status

Application Serial No. Filing Date Status

I hereby appoint the following attorney(s) and/or agent(s) to prosecute this application and to transact all business in the Patent and Trademark Office connected therewith as well as to file equivalent patent applications in countries foreign to the United States including the filing of international patent applications in accordance with the Patent Cooperation Treaty: Audley A. Ciamporcero, Jr. (Reg. #26,051), Steven P. Berman (Reg. #24,772), Andrea L. Colby (Reg. #30,194), Michael Stark (Reg. #32,495), Matthew S. Goodwin (Reg. #32,839), Dean L. Garner (Reg. #35,877), E. Richard Skula (Reg. #31,061), Bernard E. Shay (Reg. #32,061)

and Verne E. Kreger, Jr. (Reg. #35,231), One Johnson & Johnson Plaza,
New Brunswick, NJ 08933.

Address all telephone calls to Verne E. Kreger, Jr. at telephone
no. (732) 524-1239.

Address all correspondence to Audley A. Ciamporzero, Jr., One
Johnson & Johnson Plaza, New Brunswick, NJ 08933-7003.

I hereby declare that all statements made herein of my own
knowledge are true and that all statements made on information
and belief are believed to be true; and further that these
statements were made with the knowledge that willful false
statements and the like so made are punishable by fine or
imprisonment, or both, under Section 1001 of Title 18 of the
United States Code and that such willful false statements may
jeopardize the validity of the application or any patent issued
thereon.

Inventor's Signature: _____

Full Name of First Inventor

Jorg Priewe

Date: _____

Citizenship: German

Residence: Sophienblat 71 a, D-24114 Kiel, Germany

Post Office Address: same

Inventor's Signature: _____

Full Name of Second Joint Inventor Raimo Sump

Date: _____

Citizenship: German

Residence: Langenbecksh h 10, D-22337 Hamburg, Germany

Post Office Address: same

Inventor's Signature: _____

Full Name of Third Joint Inventor

Hans-Jochen Hoepffner

Date: _____

Citizenship: German

Residence: 41 Matthews Farm Road, Belle Mead, NJ 08502

Post Office Address: sam

Inventor's Signature: _____

Full Name of Third Joint Inventor

Robert J. Tannhauser

Date: _____

Citizenship: US

Residence: 265 Holland Ct., Bridgewater, NJ 08807

Post Office Address: same

09589242 " 060700